

Figure S1. Calibration curve for Cd by fluorescence spectroscopy.

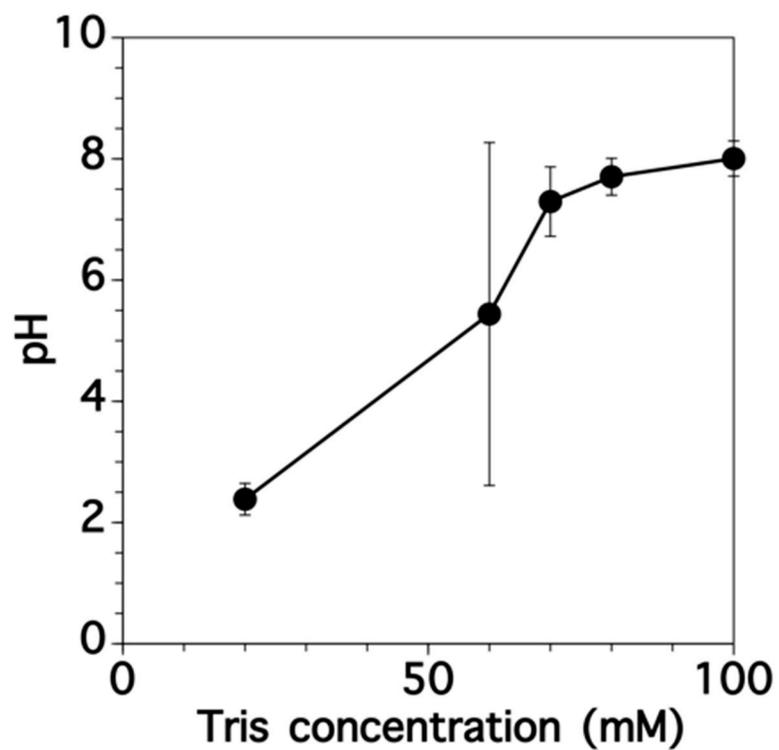


Figure S2. Effect of Tris concentration of the buffer solution on the pH of the solution under analysis.