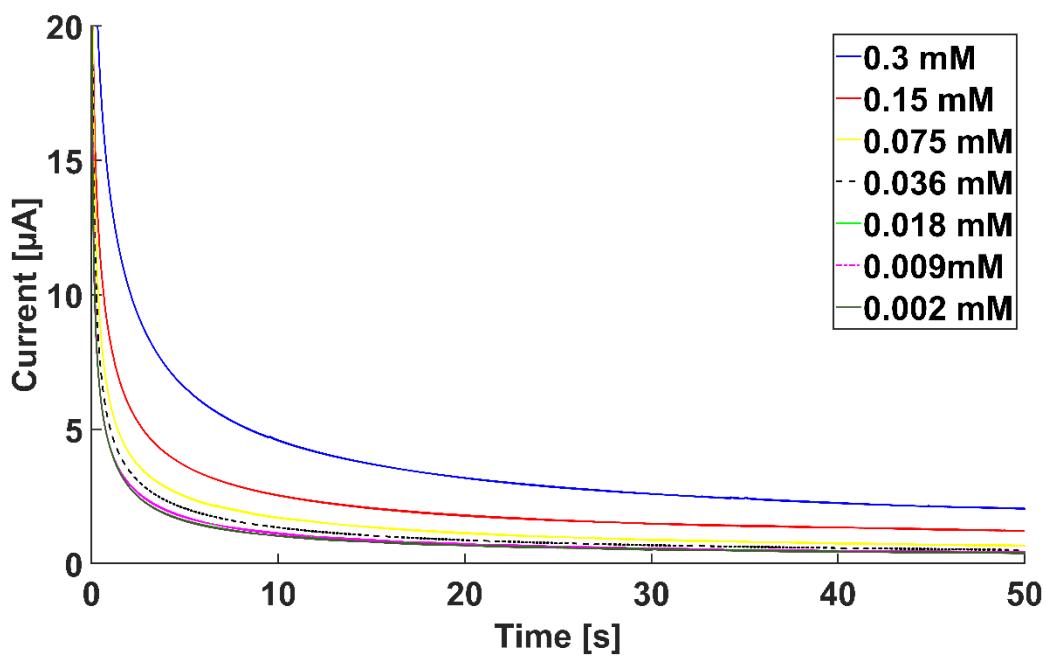


## Supplementary Material

**Table S1.** Analytical values for available ions in the water sample. Data provided by Mineral Water A/S, Denmark.

Parameter	Value	Units
Calcium	<40	mg/L
Magnesium	<15	mg/L
Sodium	<12	mg/L
Bicarbonates	<150	mg/L
Sulfate	<5	mg/L
Nitrate	<1	mg/L
Potassium	<5	mg/L
Chloride	<13	mg/L
pH	7-7.6	-



**Figure S1.** Amperometric measurements using the optimized potential of 0.78 V on different concentrations of glyphosate using a gold working electrode.