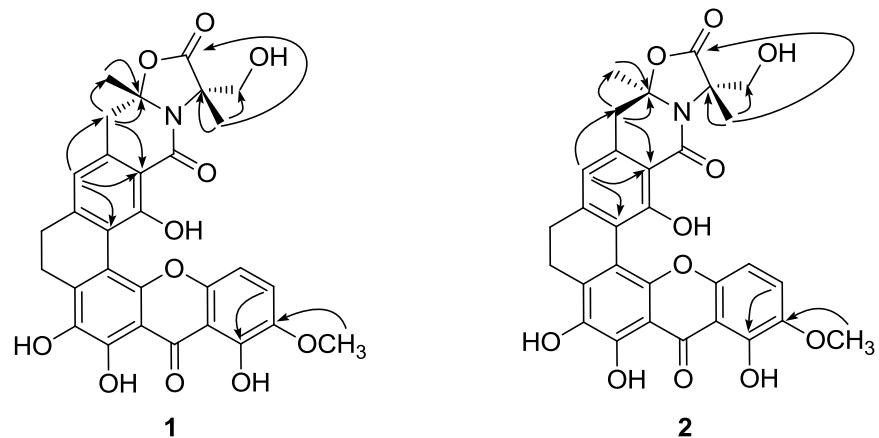
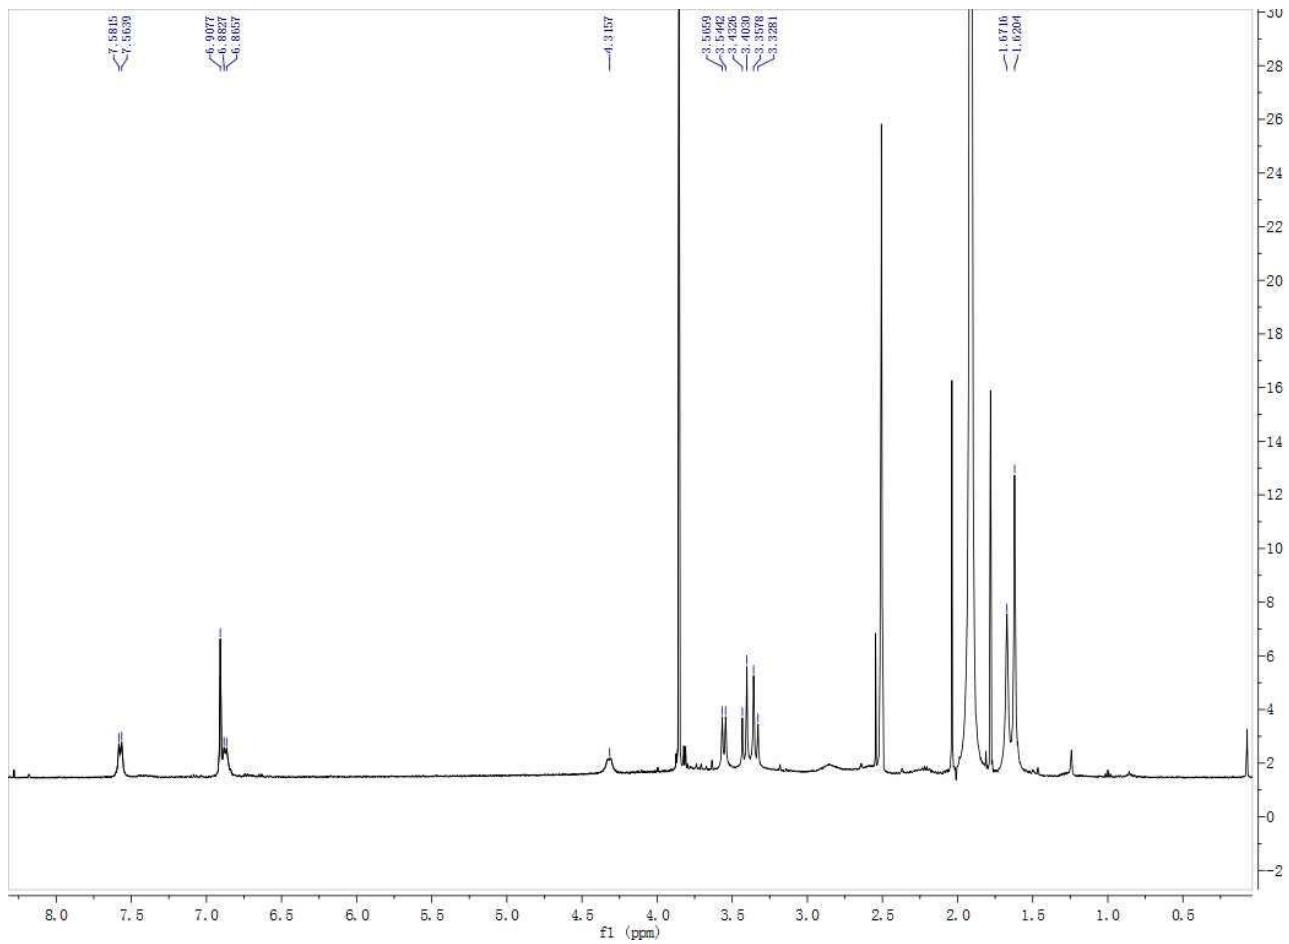
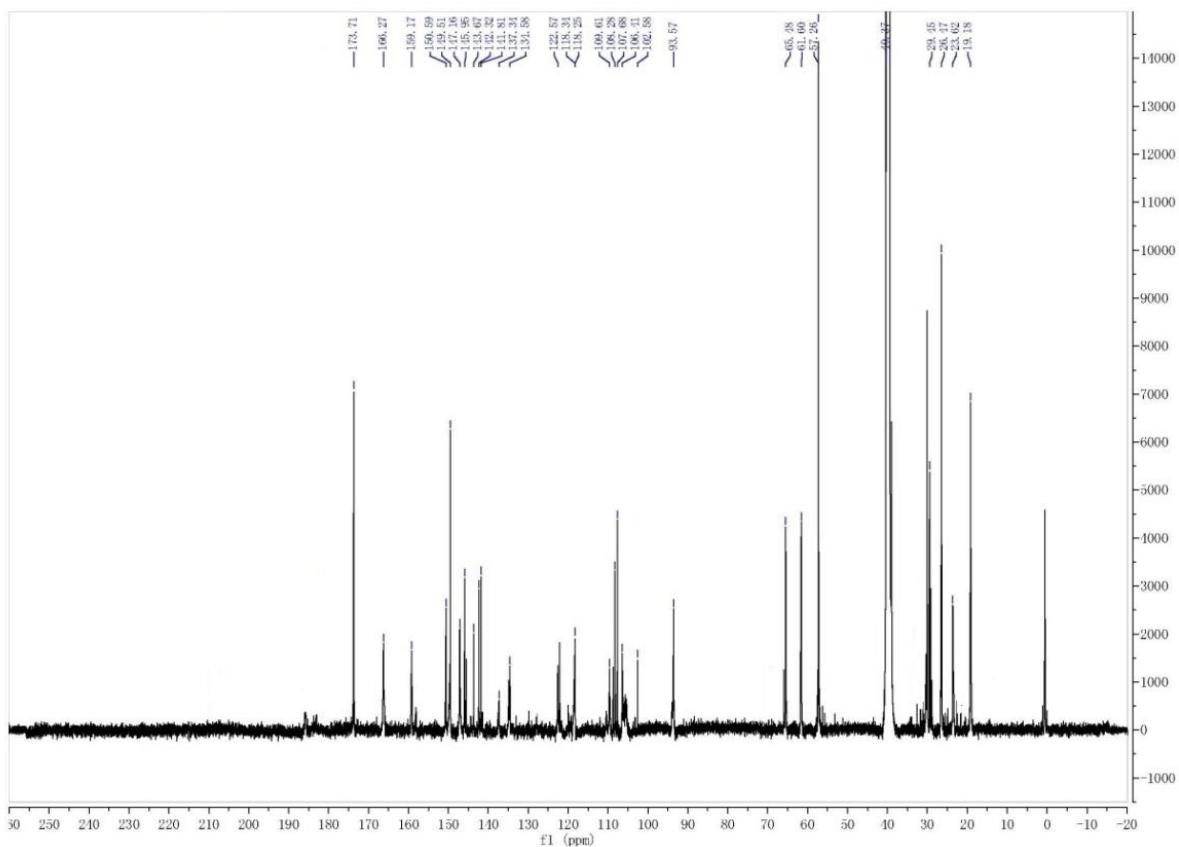
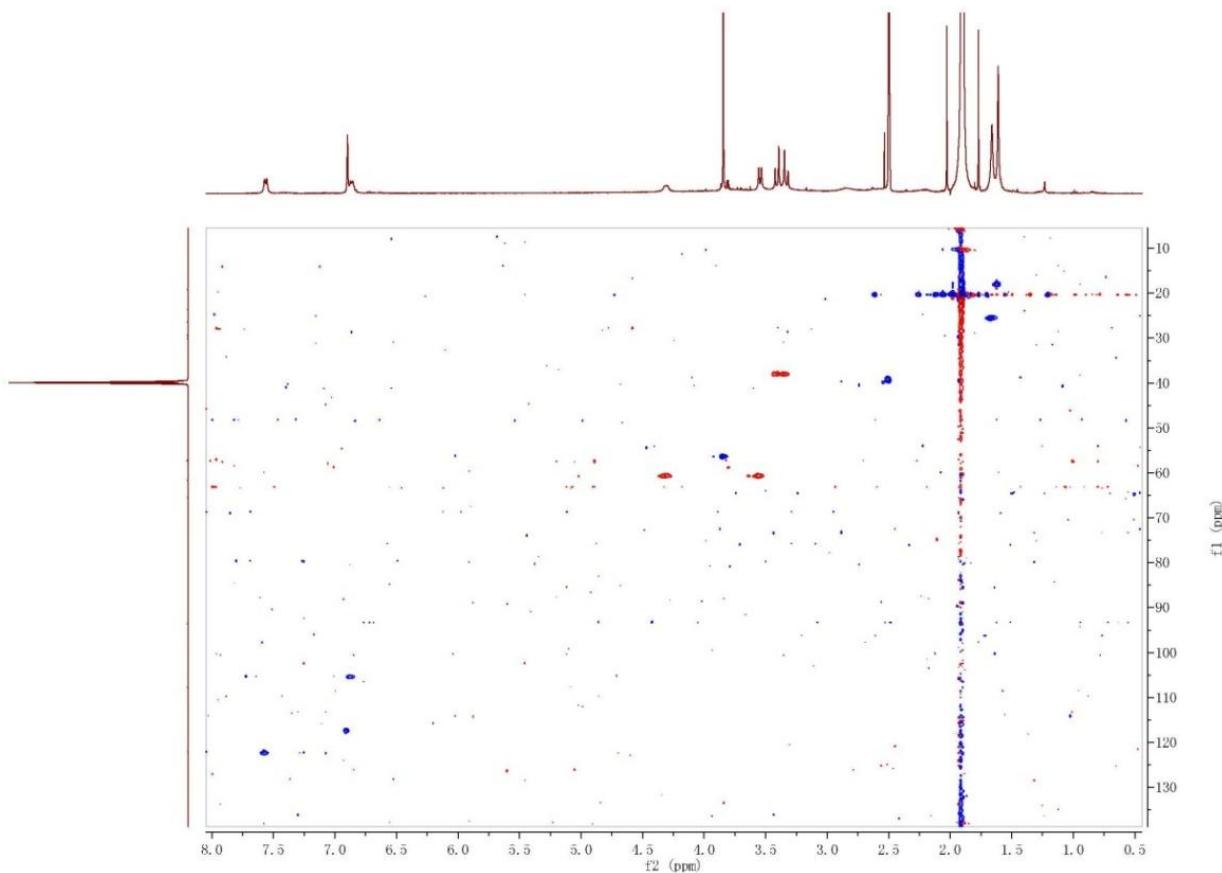
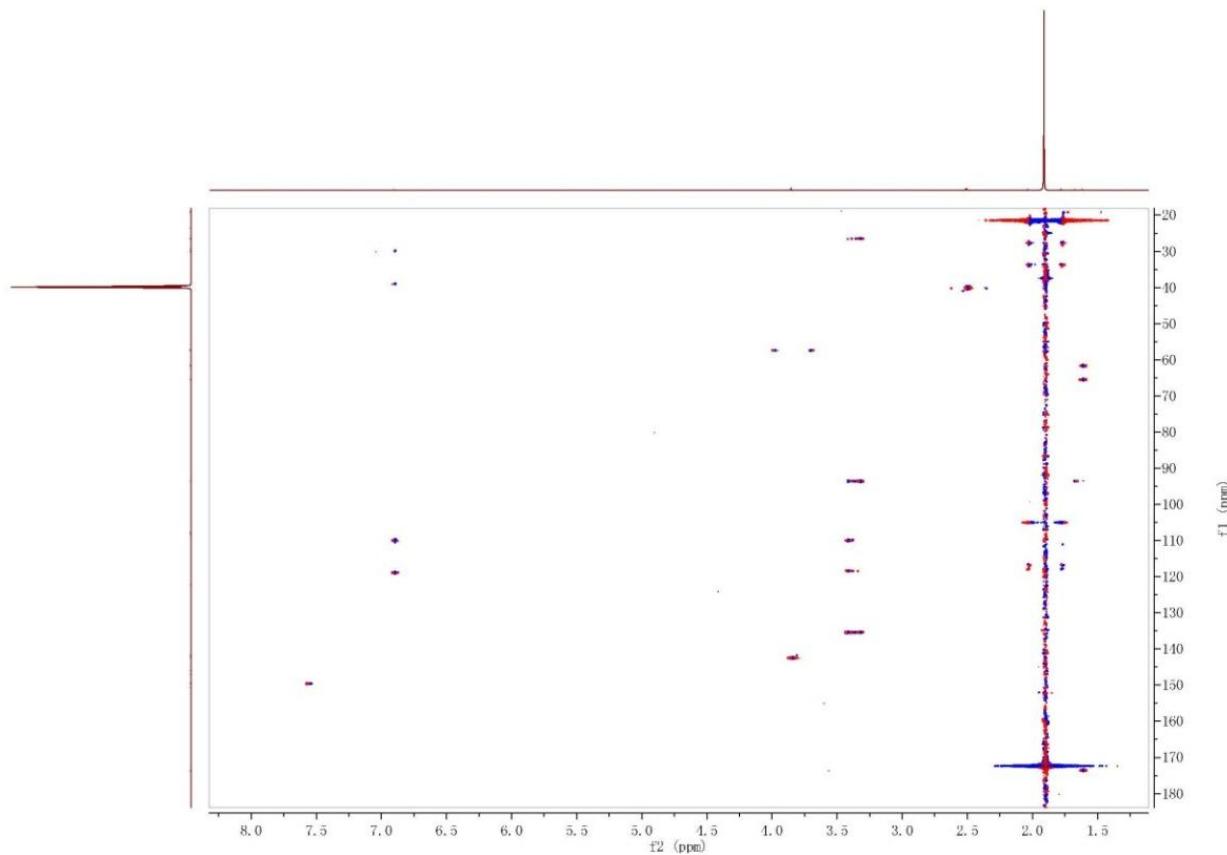
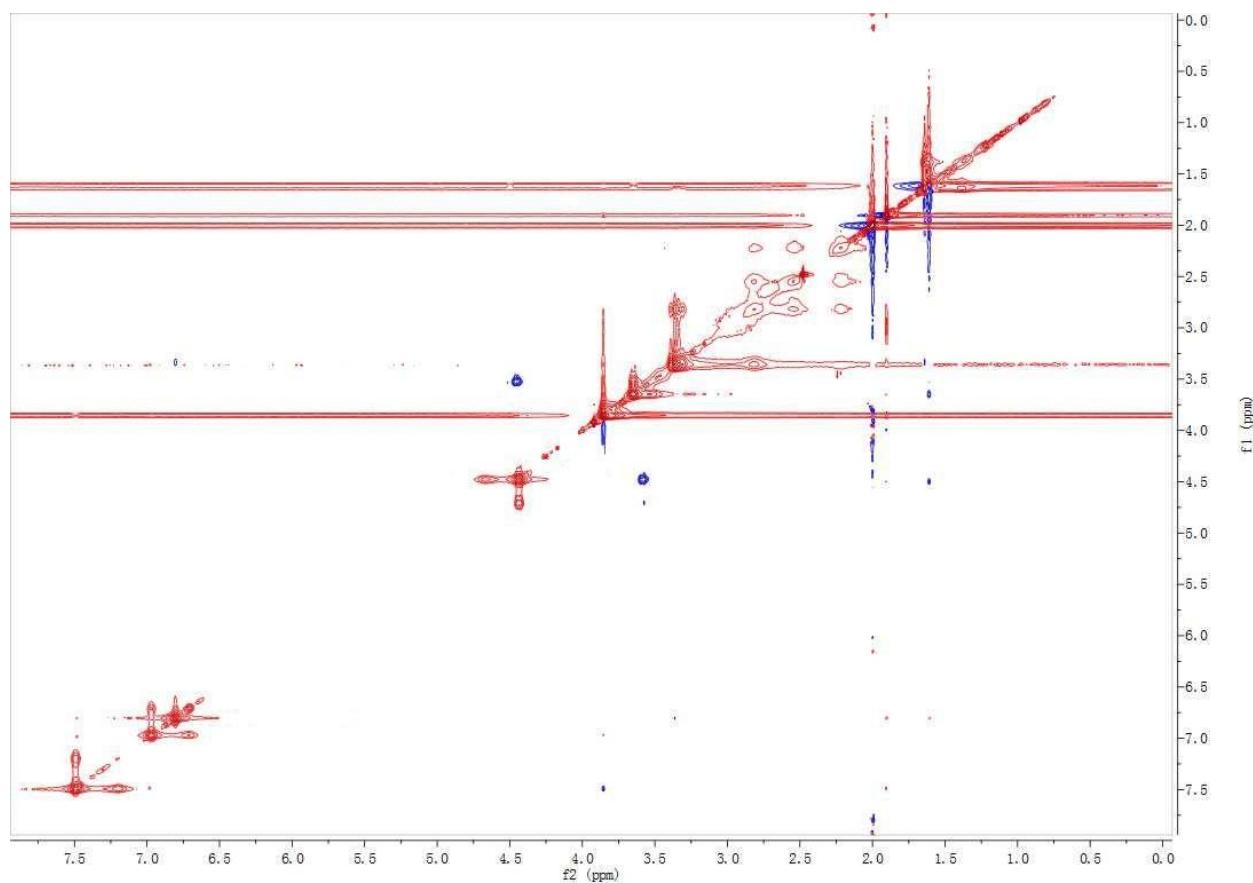


# Supplementary Information

<b>Figure S1.</b> Key HMBC correlations of compounds <b>1</b> and <b>2</b> .....	2
<b>Figure S2.</b> $^1\text{H}$ NMR spectrum of <b>1</b> in DMSO- $d_6$ .....	2
<b>Figure S3.</b> $^{13}\text{C}$ NMR spectrum of <b>1</b> in DMSO- $d_6$ .....	3
<b>Figure S4.</b> HSQC spectrum of <b>1</b> in DMSO- $d_6$ .....	3
<b>Figure S5.</b> HMBC spectrum of <b>1</b> in DMSO- $d_6$ .....	4
<b>Figure S6.</b> NOESY spectrum of <b>1</b> in DMSO- $d_6$ .....	4
<b>Figure S7.</b> HRESIMS spectrum of <b>1</b> .....	5
<b>Figure S8.</b> $^1\text{H}$ NMR spectrum of <b>2</b> in DMSO- $d_6$ .....	6
<b>Figure S9.</b> $^{13}\text{C}$ NMR spectra of <b>2</b> in DMSO- $d_6$ .....	6
<b>Figure S10.</b> HSQC spectrum of <b>2</b> in DMSO- $d_6$ .....	7
<b>Figure S11.</b> HMBC spectrum of <b>2</b> in DMSO- $d_6$ .....	7
<b>Figure S12.</b> NOESY spectrum of <b>2</b> in DMSO- $d_6$ .....	8
<b>Figure S13.</b> HRESIMS spectrum of <b>2</b> .....	9
<b>Figure S14.</b> 3D mode and the key NOE correlations of compounds <b>1</b> and <b>2</b> .....	10
<b>Figure S15.</b> $^1\text{H}$ NMR spectrum of <b>3</b> in DMSO- $d_6$ .....	11
<b>Figure S16.</b> $^{13}\text{C}$ NMR spectrum of <b>3</b> in DMSO- $d_6$ .....	11
<b>Figure S17.</b> HSQC spectrum of <b>3</b> in DMSO- $d_6$ .....	12
<b>Figure S18.</b> HMBC spectrum of <b>3</b> in DMSO- $d_6$ .....	12
<b>Figure S19.</b> HRESIMS spectrum of <b>3</b> .....	13
<b>Figure S20.</b> $^1\text{H}$ NMR spectrum of <b>4</b> in DMSO- $d_6$ .....	14
<b>Figure S21.</b> $^{13}\text{C}$ NMR spectrum of <b>4</b> in DMSO- $d_6$ .....	14
<b>Figure S22.</b> HSQC spectrum of <b>4</b> in DMSO- $d_6$ .....	15
<b>Figure S23.</b> HRESIMS spectrum of <b>4</b> .....	15
<b>Figure S24.</b> HRESIMS spectrum of <b>4</b> .....	16

**Figure S1.** Key HMBC correlations of compounds **1** and **2**.**Figure S2.**  $^1\text{H}$  NMR spectrum of **1** in  $\text{DMSO}-d_6$ .

**Figure S3.**  $^{13}\text{C}$  NMR spectrum of **1** in  $\text{DMSO}-d_6$ .**Figure S4.** HSQC spectrum of **1** in  $\text{DMSO}-d_6$ .

**Figure S5.** HMBC spectrum of **1** in DMSO-*d*<sub>6</sub>.**Figure S6.** NOESY spectrum of **1** in DMSO-*d*<sub>6</sub>.

**Figure S7.** HRESIMS spectrum of **1**.

## Display Report

**Analysis Info**


Analysis Name G:\leonie-MS\0803\AM-5A\_1-C,2\_01\_3348.d  
 Method LC-5%-ms-pos.m  
 Sample Name AM-5A  
 Comment



Acquisition Date 8/3/2011 6:42:48 PM



Operator BDAL@DE  
 Instrument / Ser# micrOTOF 10249


**Acquisition Parameter**

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	4.0 Bar
Focus	Active			Set Dry Heater	200 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	8.0 l/min
Scan End	1500 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Waste

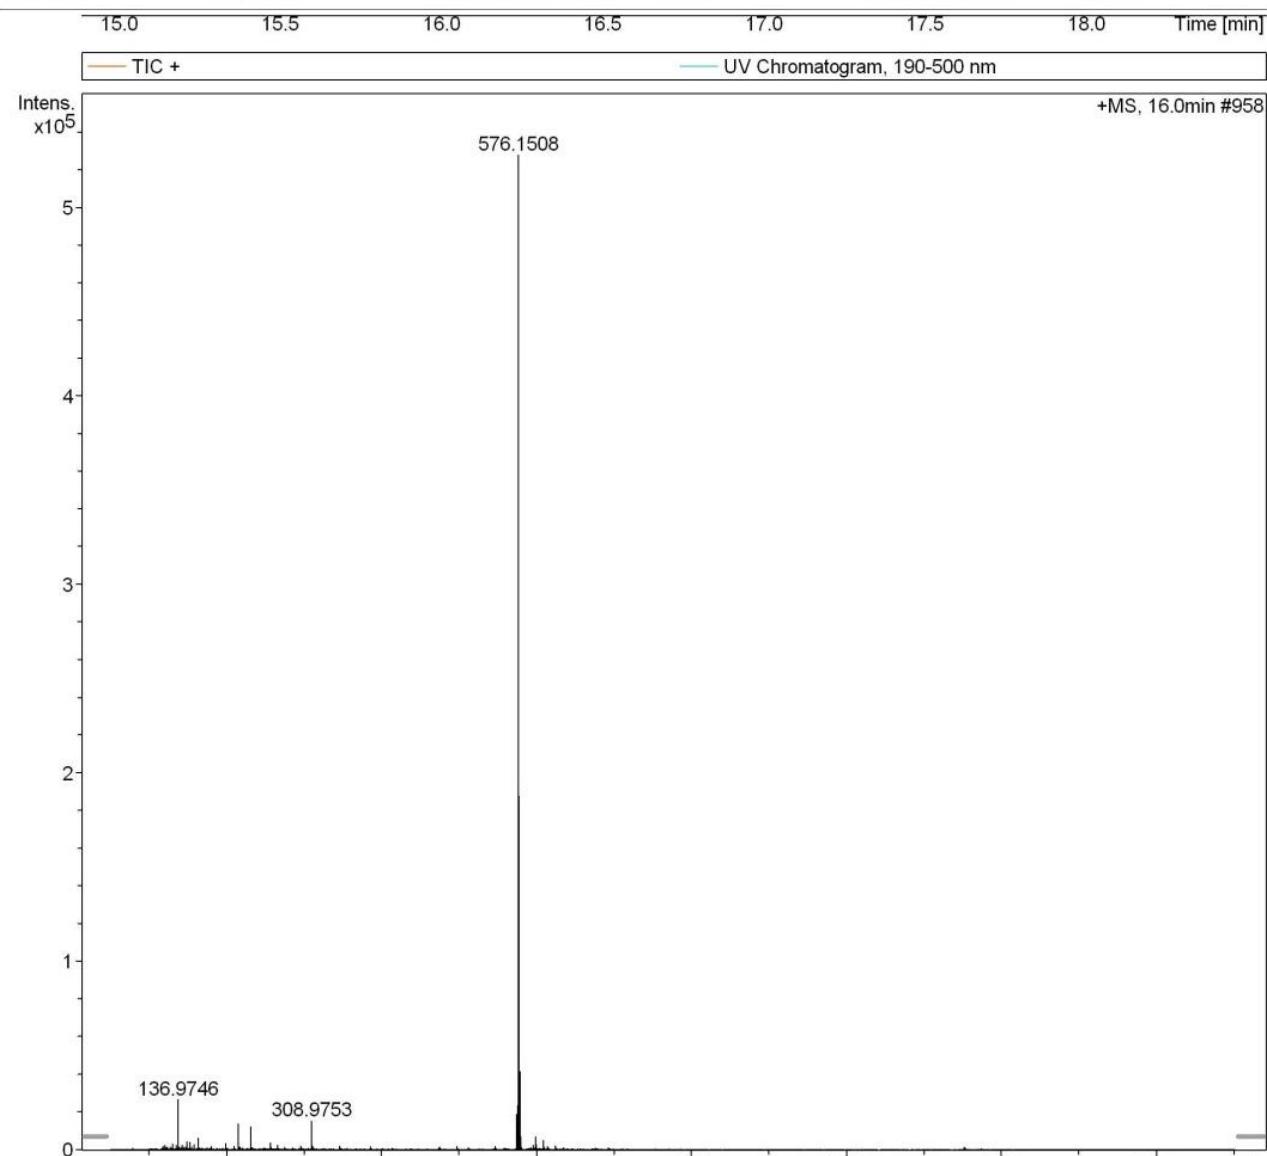

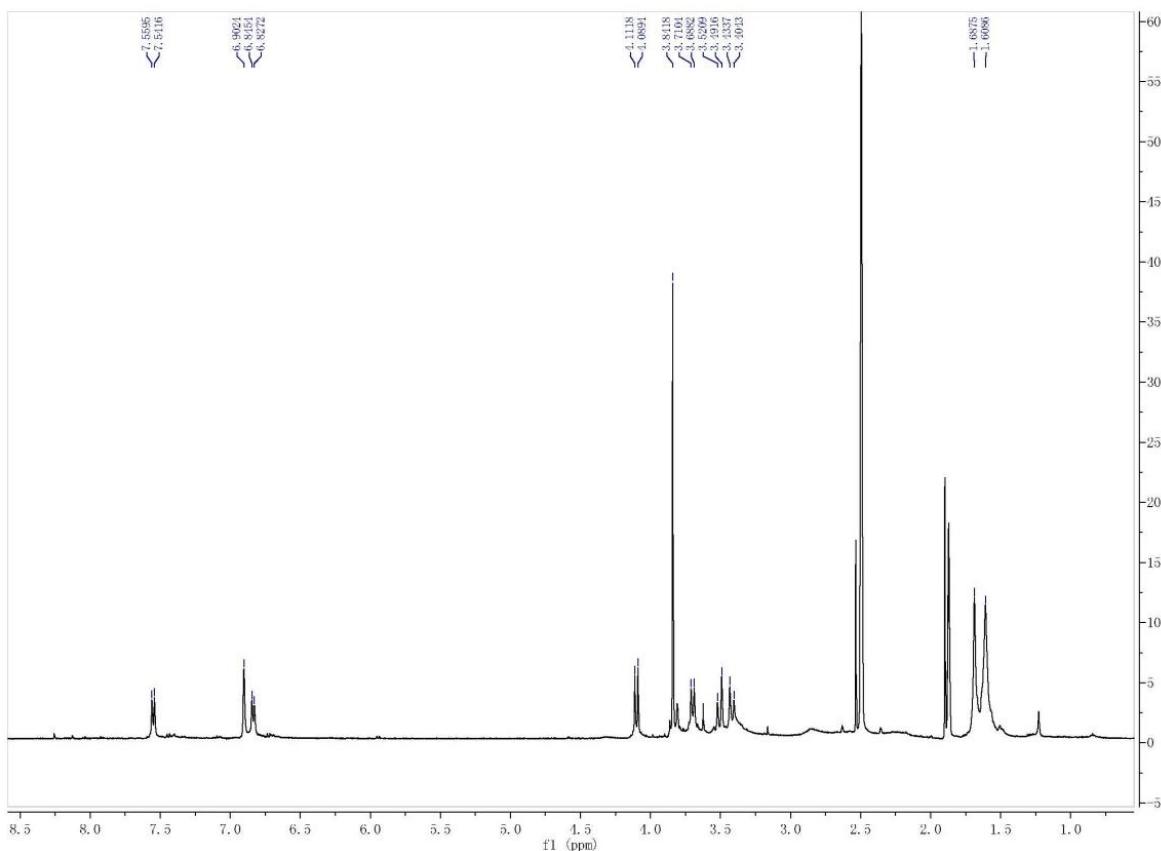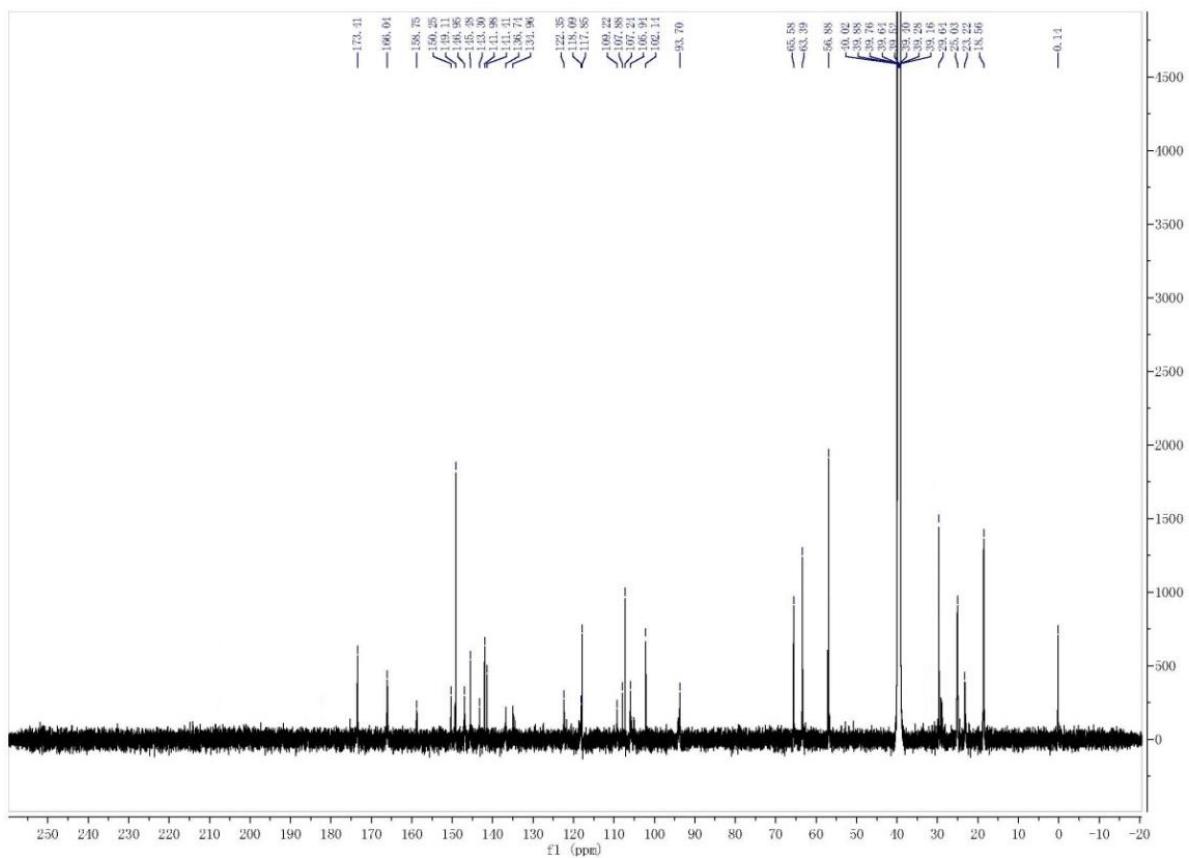**Figure S8.**  $^1\text{H}$  NMR spectrum of **2** in  $\text{DMSO}-d_6$ .**Figure S9.**  $^{13}\text{C}$  NMR spectra of **2** in  $\text{DMSO}-d_6$ .

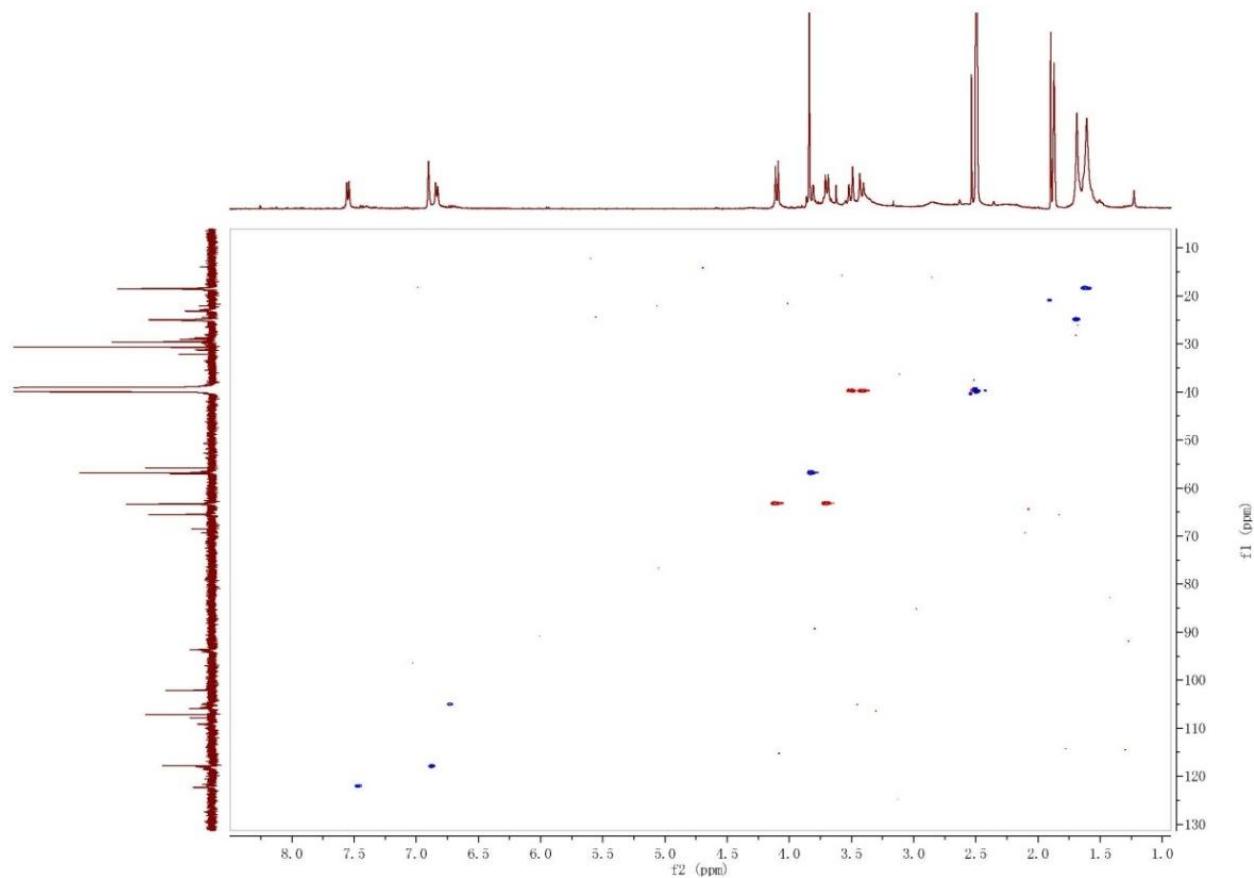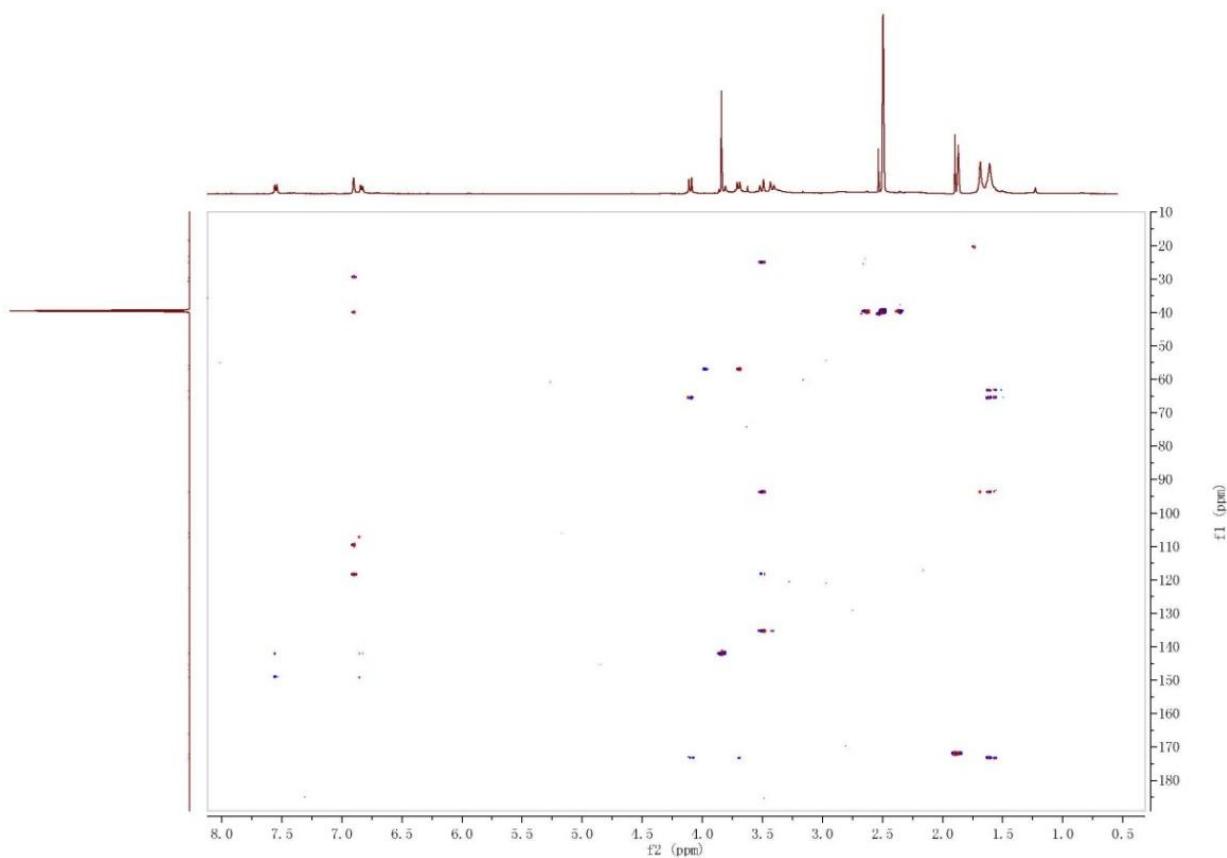**Figure S10.** HSQC spectrum of **2** in DMSO-*d*<sub>6</sub>.**Figure S11.** HMBC spectrum of **2** in DMSO-*d*<sub>6</sub>.

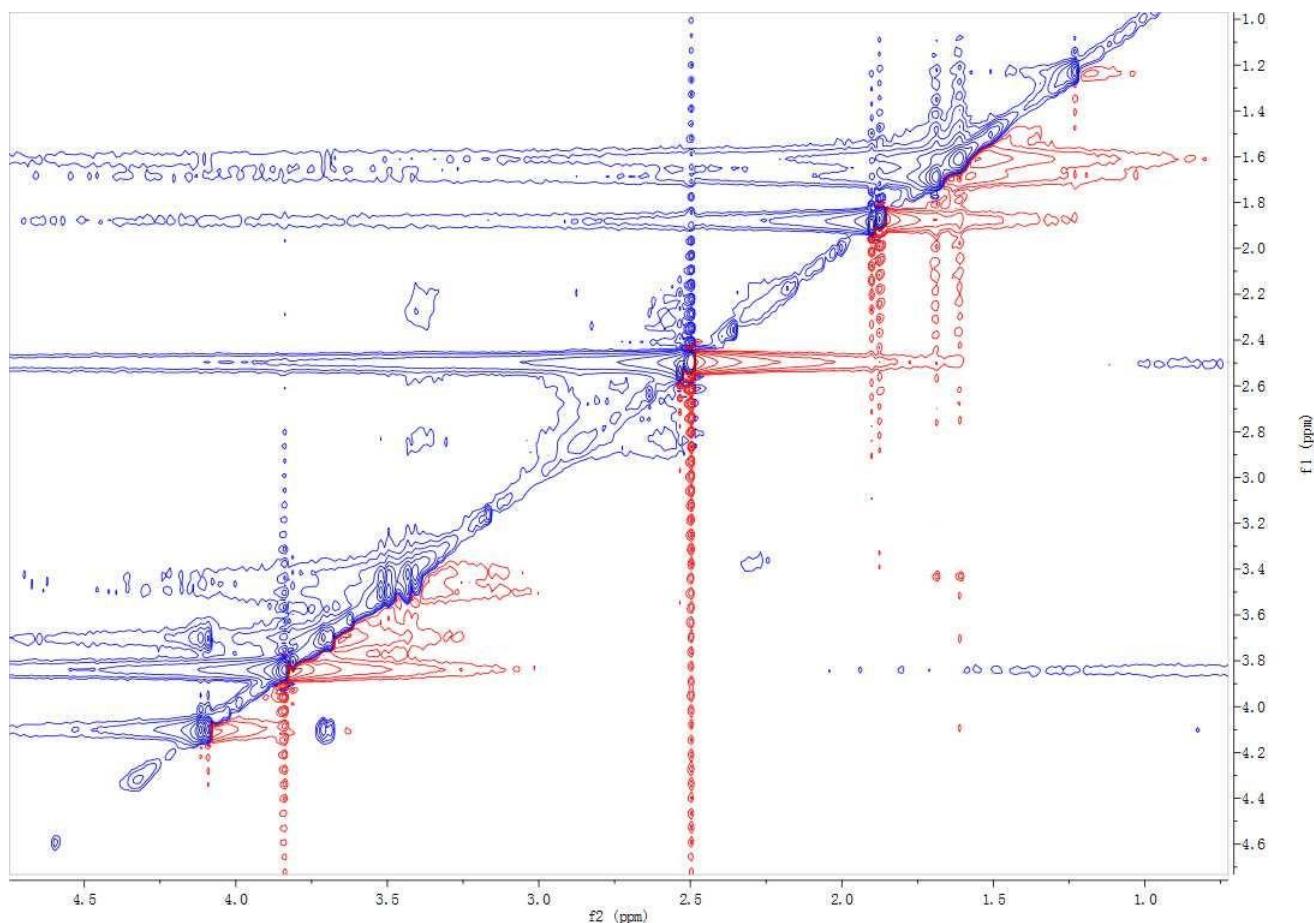**Figure S12.** NOESY spectrum of **2** in DMSO-*d*<sub>6</sub>.

**Figure S13.** HRESIMS spectrum of 2.

## Display Report


**Analysis Info**

Analysis Name G:\leonie-MS\0803\AM-6A\_1-C,3\_01\_3349.d  
 Method LC-5%-ms-pos.m  
 Sample Name AM-6A  
 Comment


Acquisition Date 8/3/2011 7:11:06 PM

Operator BDAL@DE  
 Instrument / Ser# micrOTOF 10249**Acquisition Parameter**


Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	4.0 Bar
Focus	Active			Set Dry Heater	200 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	8.0 l/min
Scan End	1500 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Waste

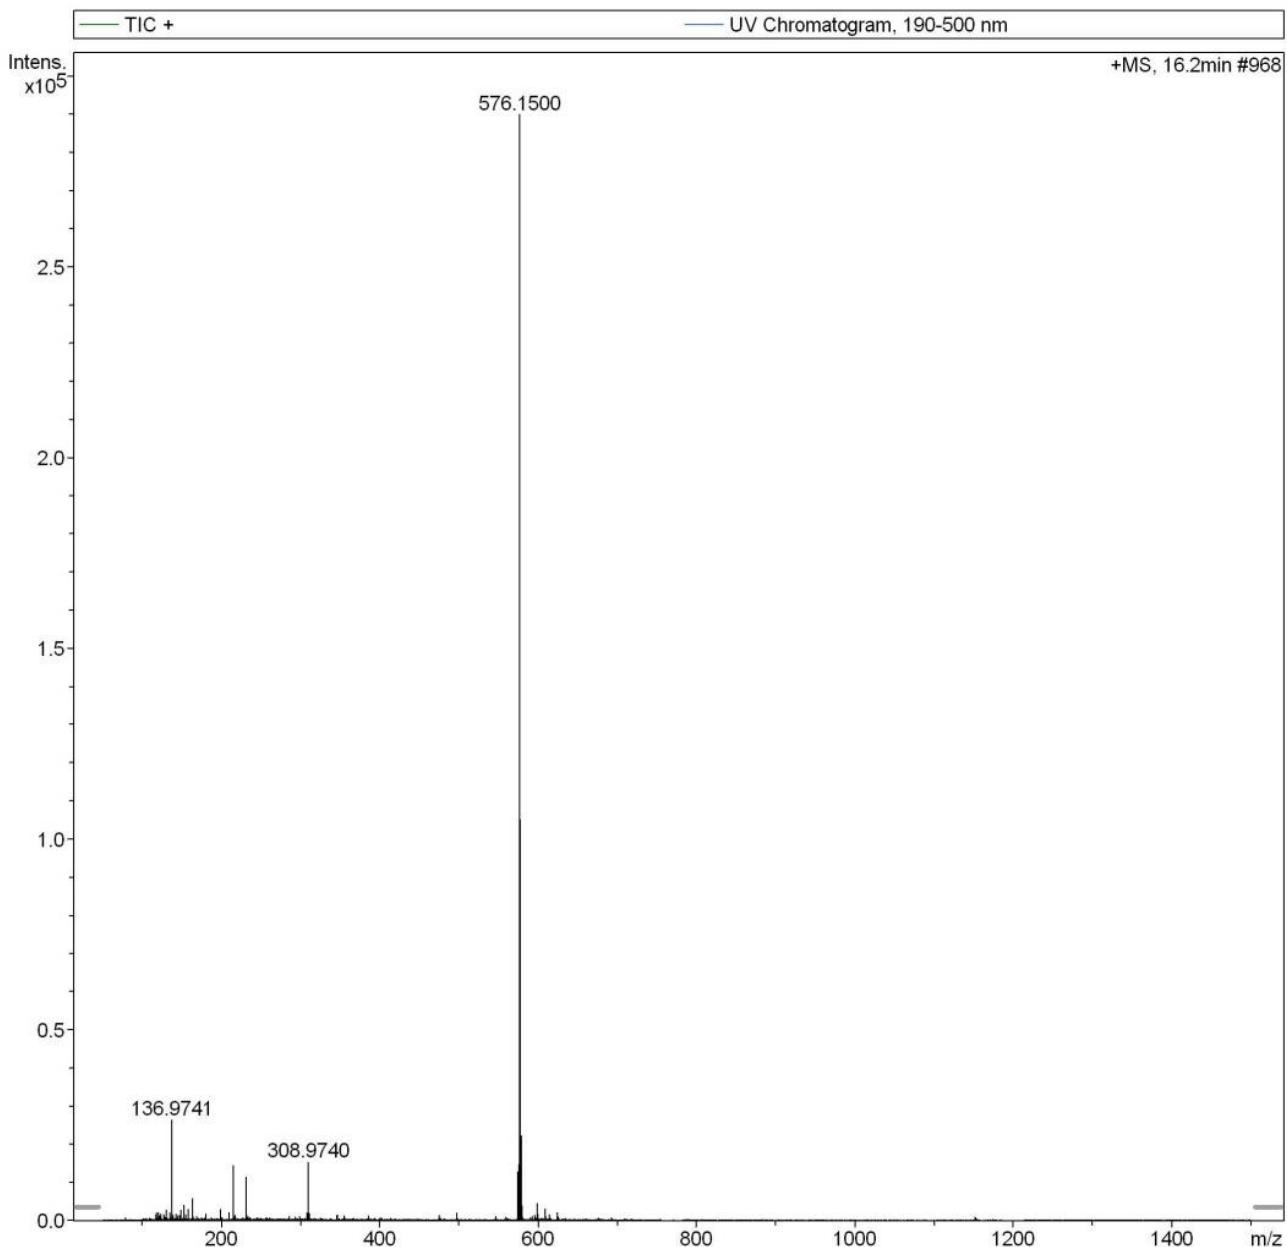


**Figure S14.** 3D mode and key NOE correlations of compounds **1** and **2**. The structures of compounds **1** and **2** have been optimized by the MM2 force field.


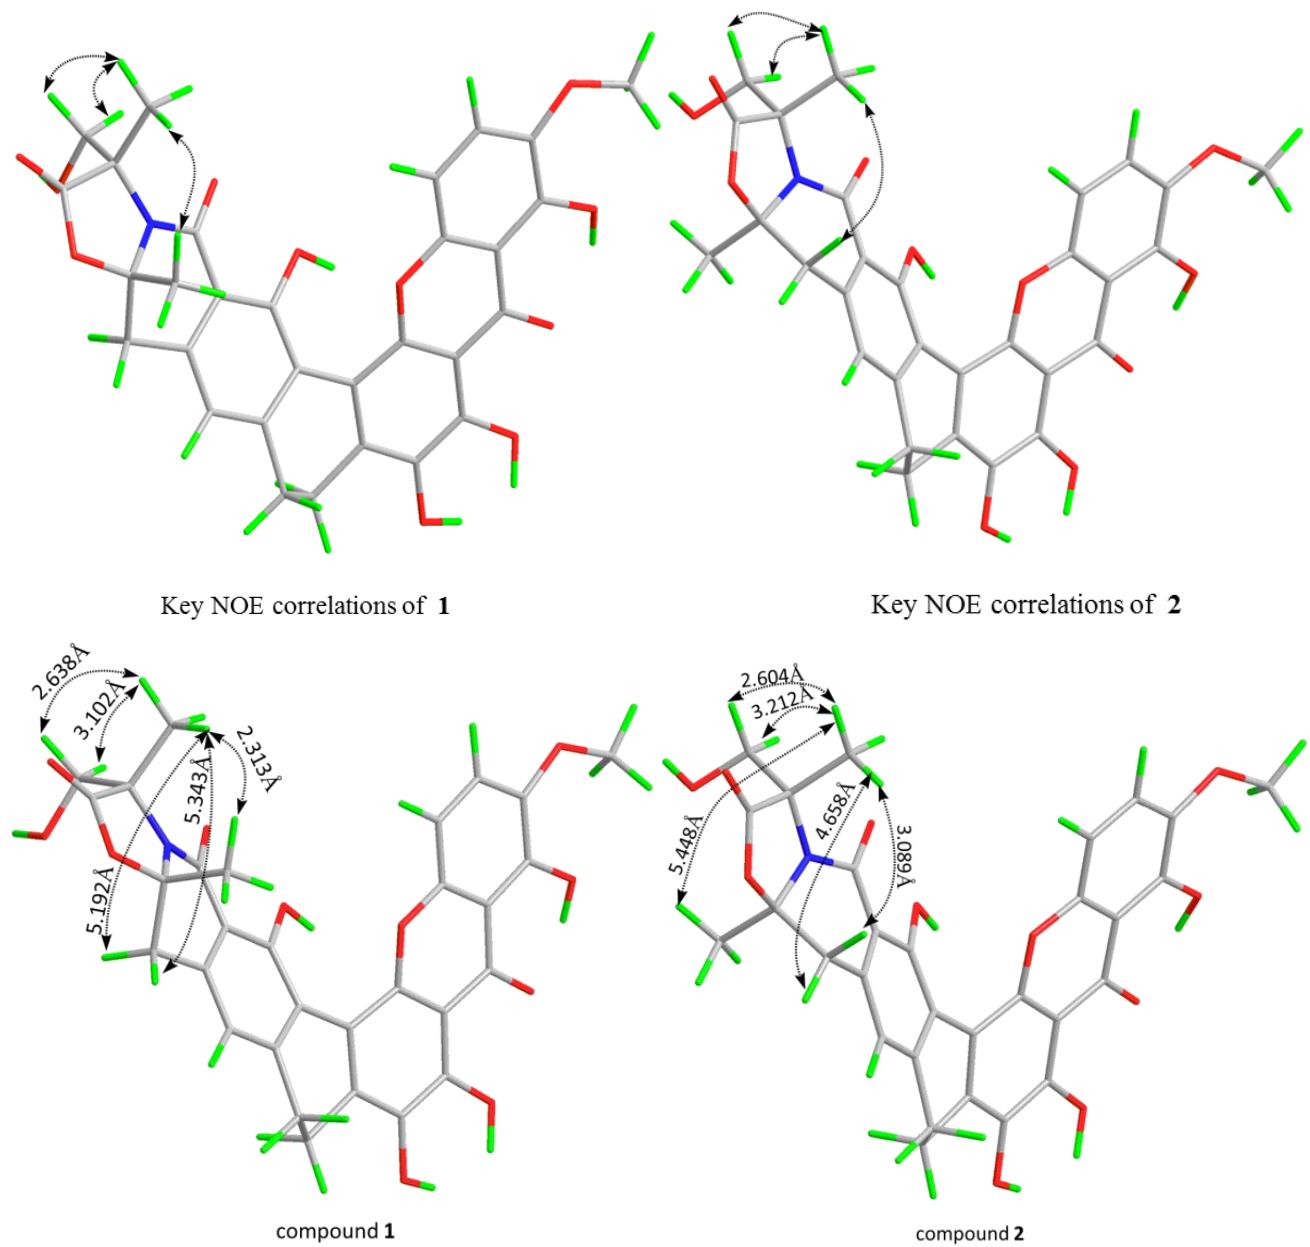


**Figure S15.**  $^1\text{H}$  NMR spectrum of **3** in  $\text{DMSO}-d_6$ .

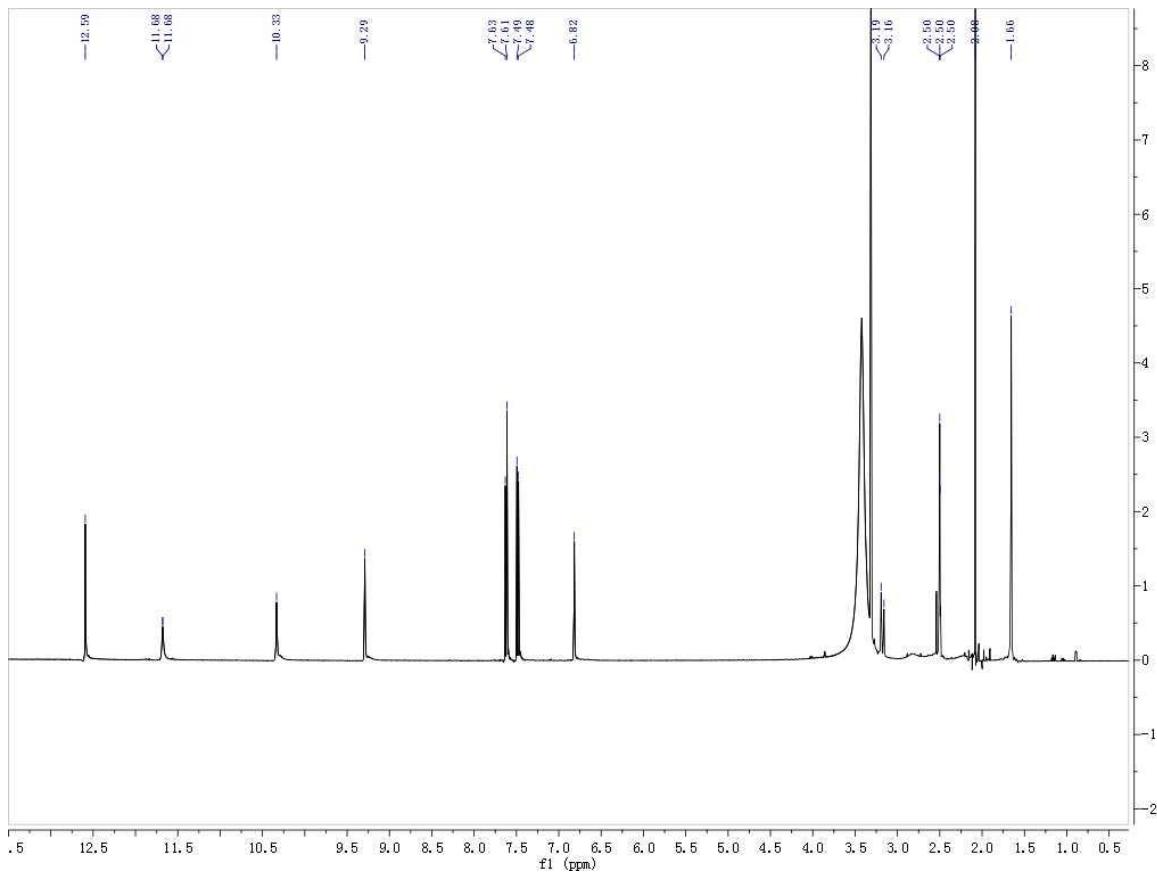

**Figure S16.**  $^{13}\text{C}$  NMR spectrum of **3** in  $\text{DMSO}-d_6$ .

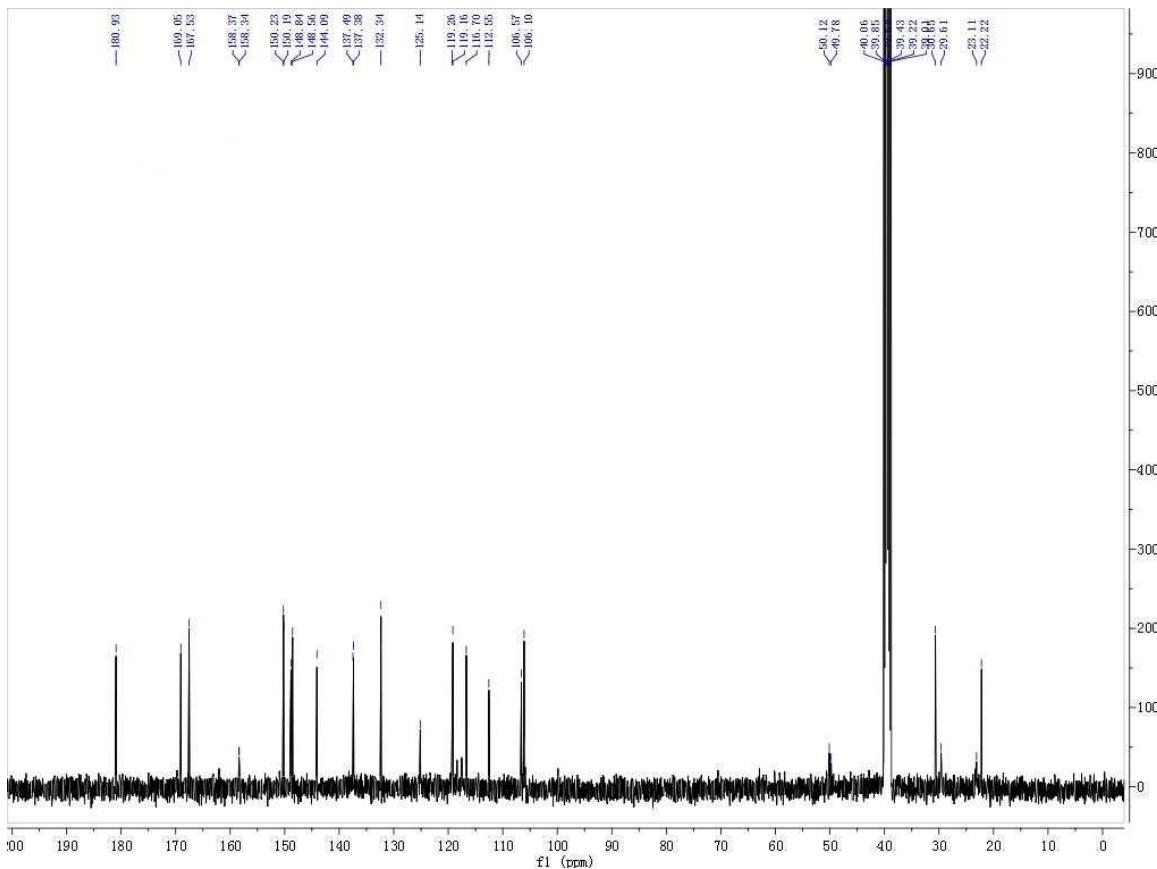

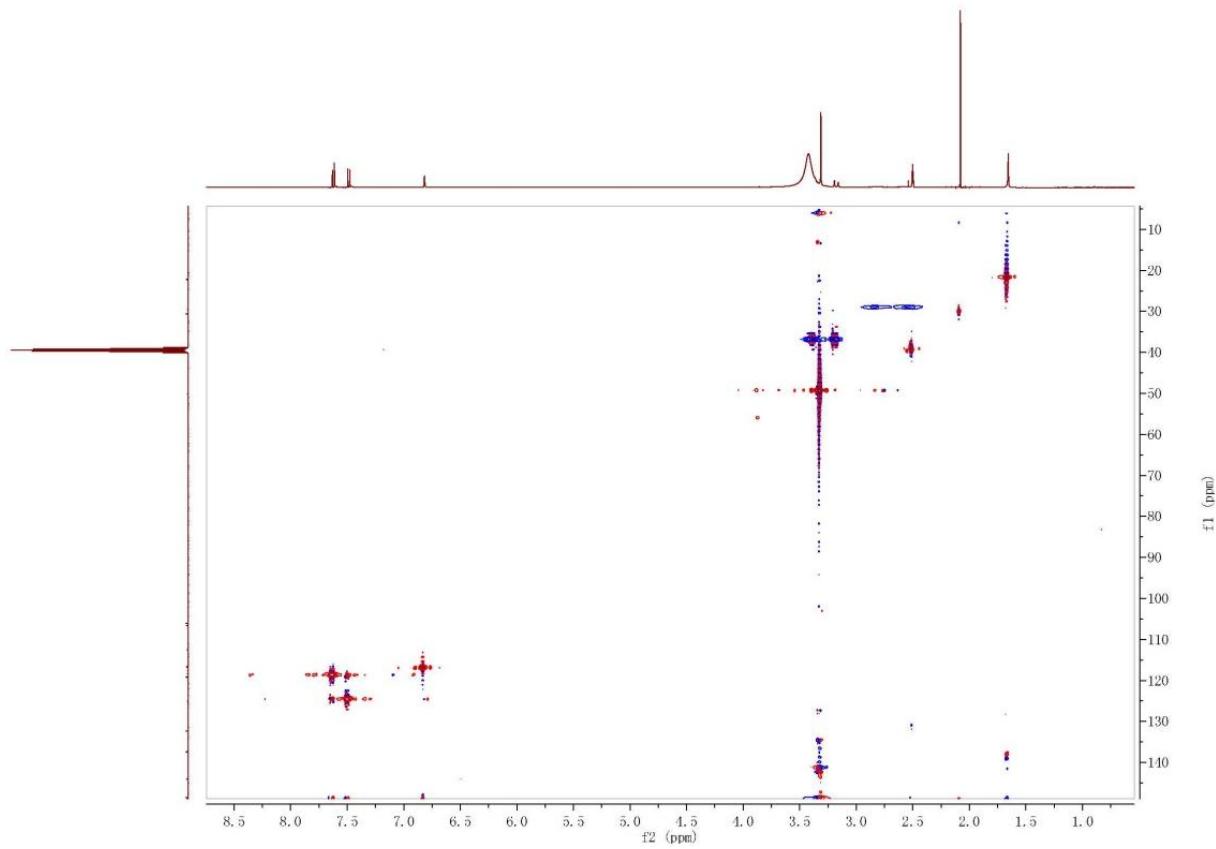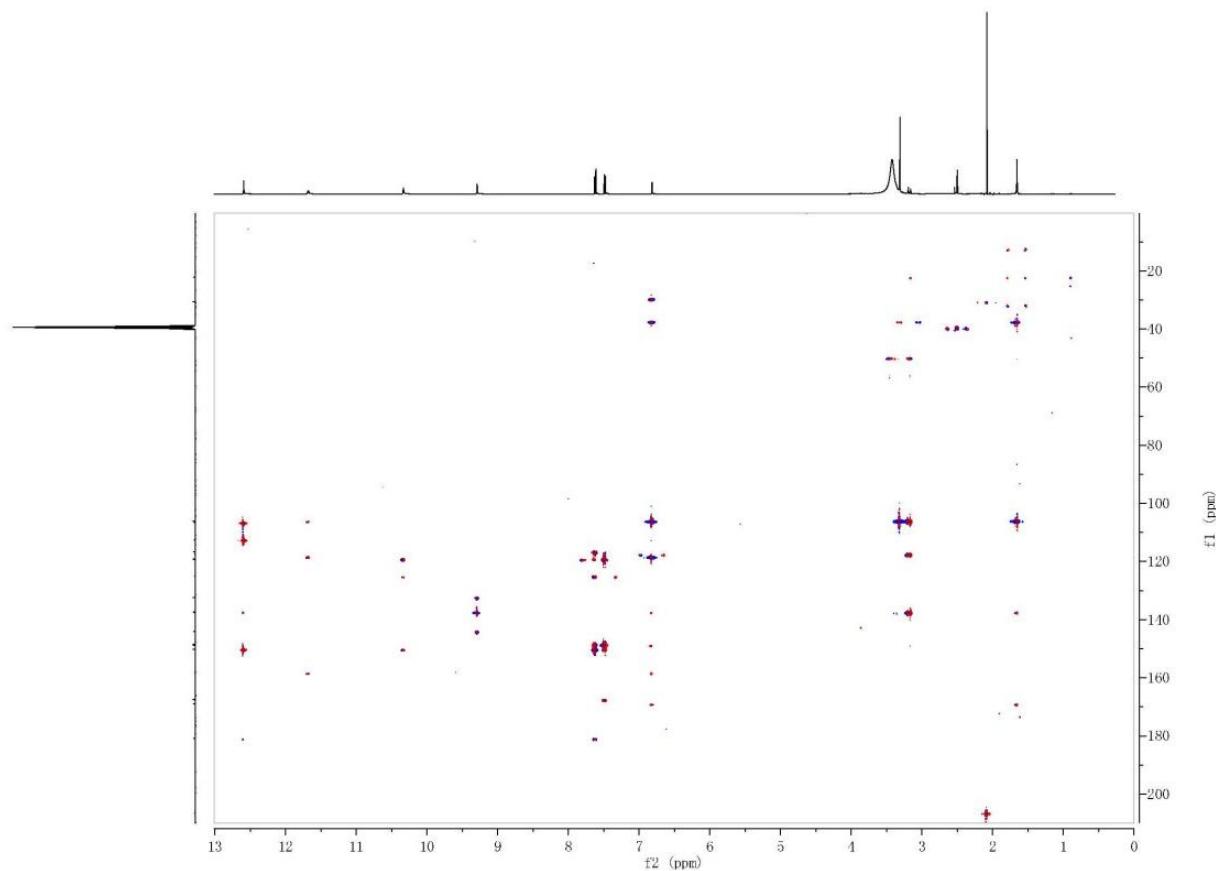**Figure S17.** HSQC spectrum of **3** in DMSO-*d*<sub>6</sub>.**Figure S18.** HMBC spectrum of **3** in DMSO-*d*<sub>6</sub>.

**Figure S19.** HRESIMS spectrum of **3**.

---

## Display Report

---


**Analysis Info**



Analysis Name G:\leonie-MS\LLL-am-8\AM-8\_1-C,1\_01\_3031.d  
 Method LC-MS-5%.m  
 Sample Name AM-8  
 Comment



Acquisition Date 5/16/2011 11:14:55 PM

Operator BDAL@DE  
 Instrument / Ser# micrOTOF 10249**Acquisition Parameter**

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	4.0 Bar
Focus	Active			Set Dry Heater	200 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	8.0 l/min
Scan End	1500 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Waste

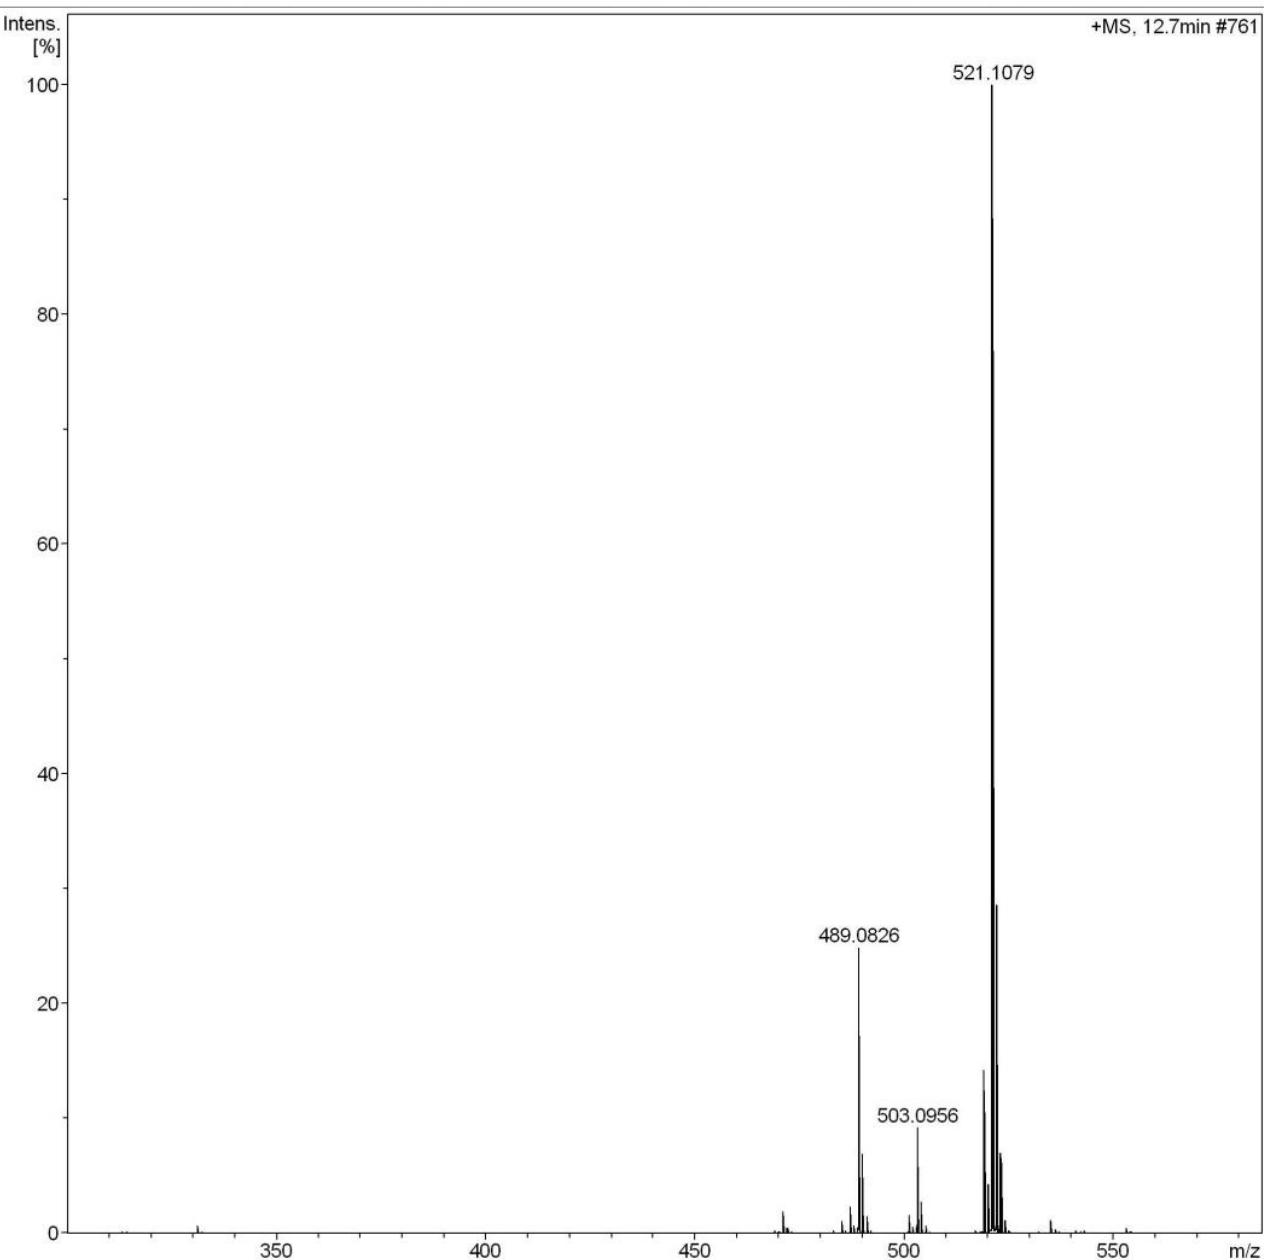

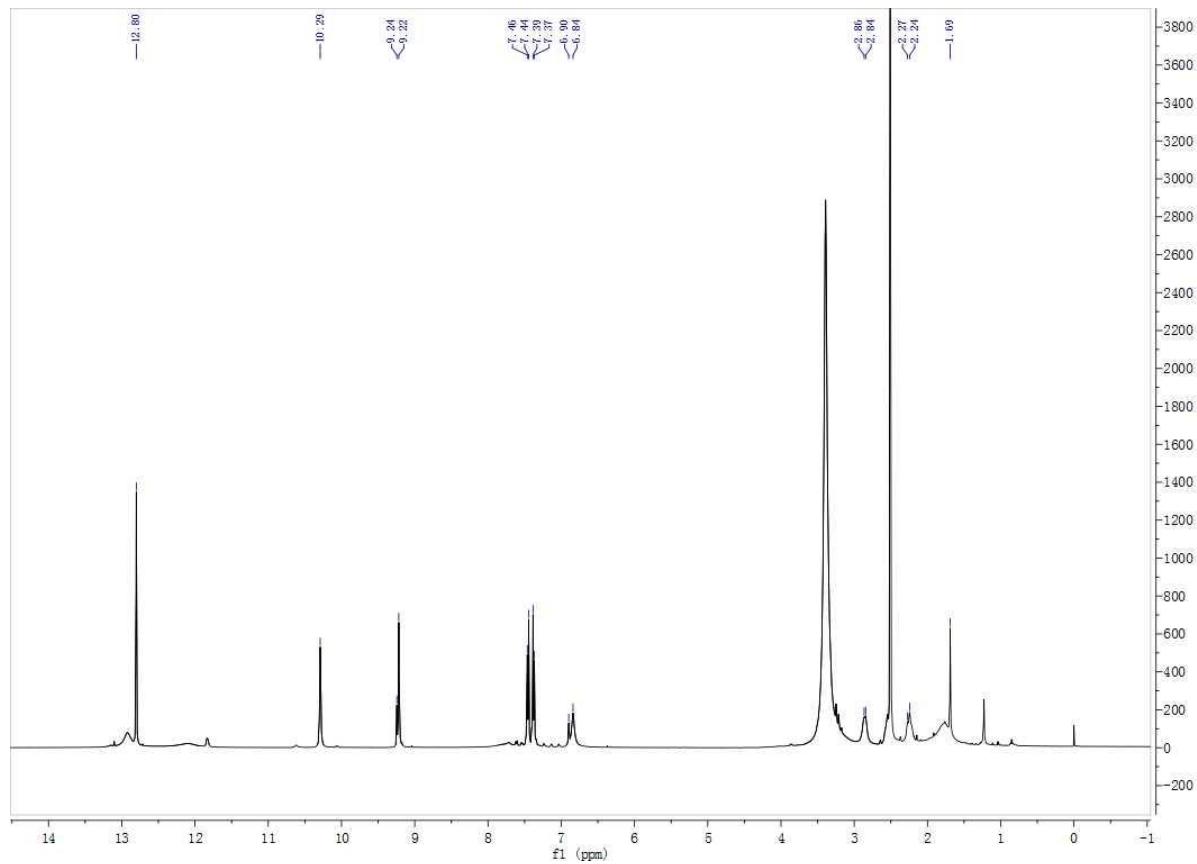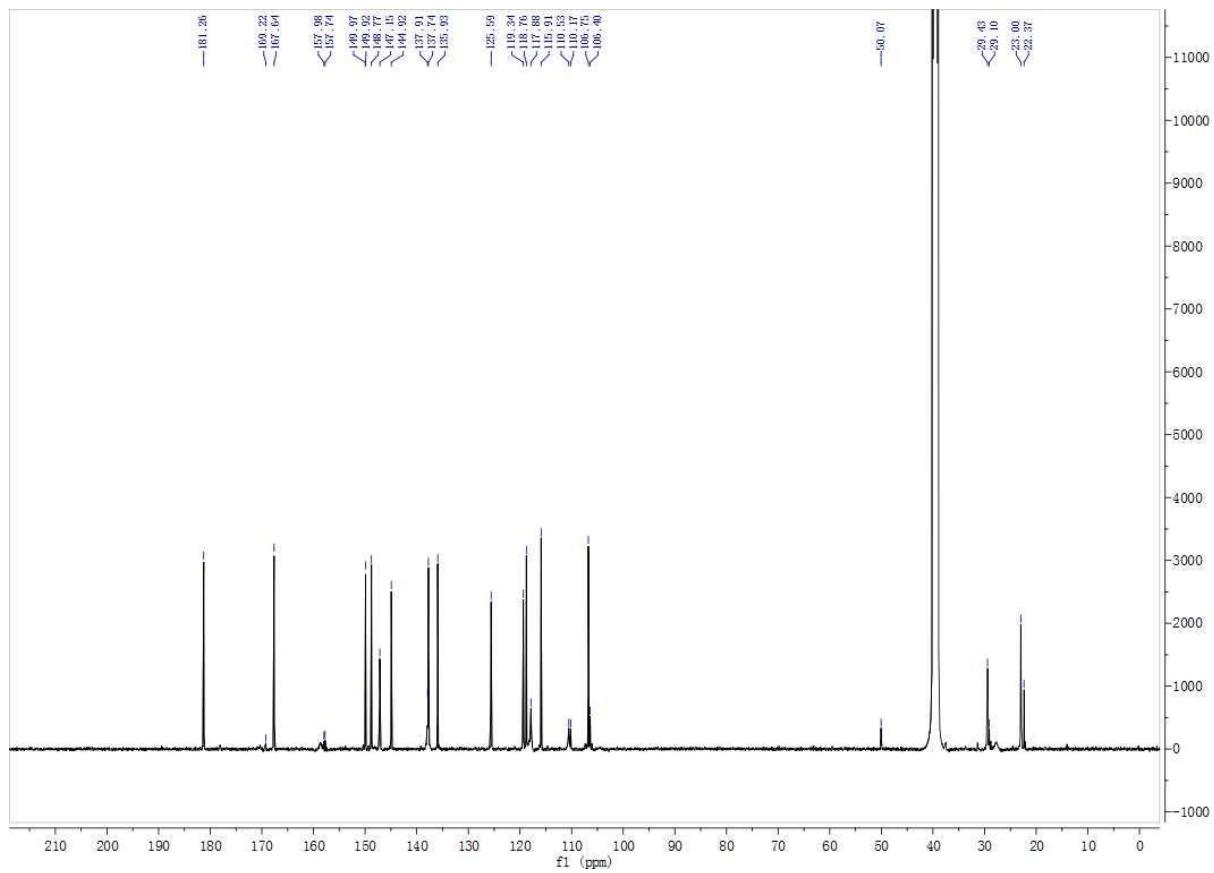**Figure S20.**  $^1\text{H}$  NMR spectrum of **4** in  $\text{DMSO}-d_6$ .**Figure S21.**  $^{13}\text{C}$  NMR spectrum of **4** in  $\text{DMSO}-d_6$ .

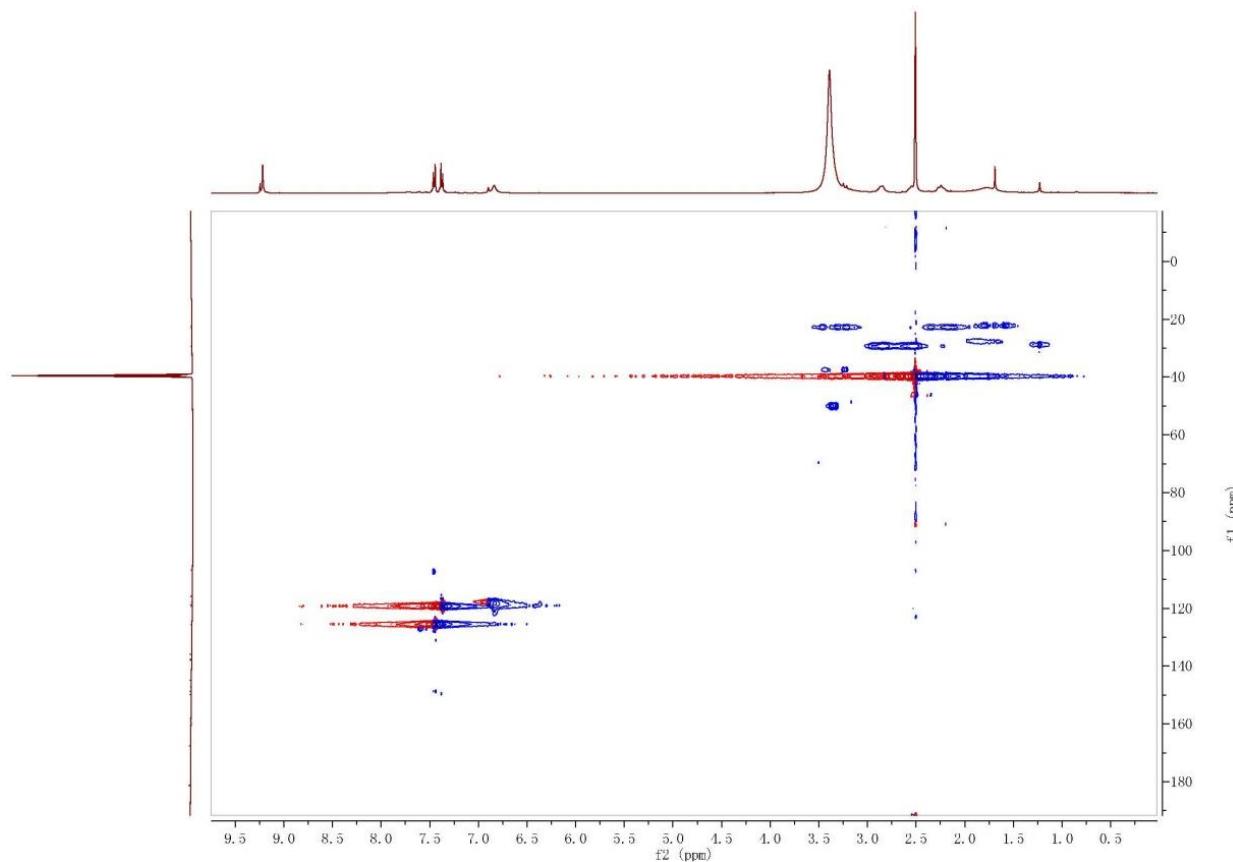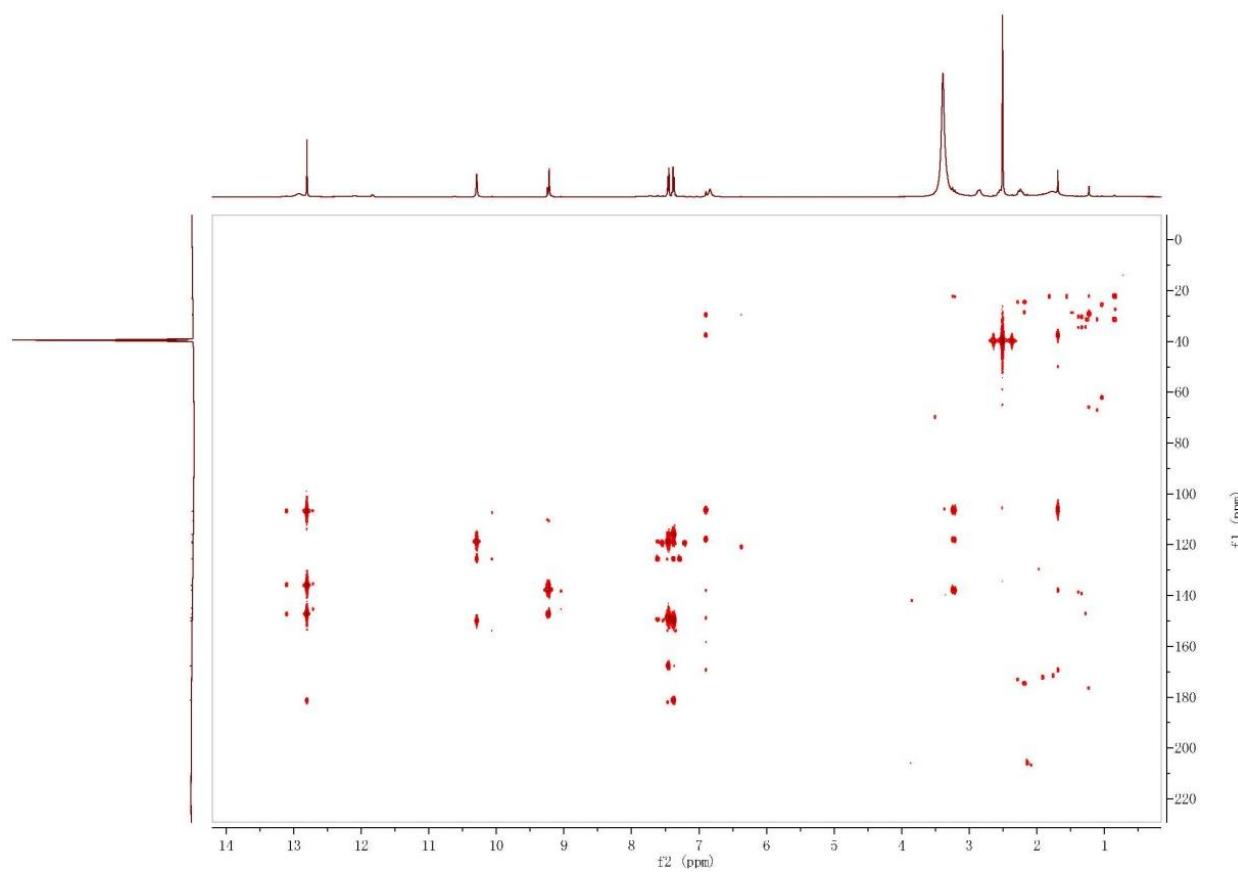**Figure S22.** HSQC spectrum of **4** in DMSO-*d*<sub>6</sub>.**Figure S23.** HMBC spectrum of **4** in DMSO-*d*<sub>6</sub>.

**Figure S24.** HRESIMS spectrum of 4.

---

## Display Report

---

**Analysis Info**

Analysis Name G:\leonie-MS\Am-13\_1-C,4\_01\_3059.d  
 Method LC-MS-5%.m  
 Sample Name Am-13  
 Comment

Acquisition Date 5/27/2011 9:26:12 PM

Operator BDAL@DE  
 Instrument / Ser# micrOTOF 10249**Acquisition Parameter**

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	4.0 Bar
Focus	Active			Set Dry Heater	200 °C
Scan Begin	50 m/z	Set Capillary	4500 V	Set Dry Gas	8.0 l/min
Scan End	1500 m/z	Set End Plate Offset	-500 V	Set Divert Valve	Waste

