

Table S1: Intra-Day and Inter-Day Accuracy and Precision for the Determination of GSH by the Proposed HPLC Procedure:

Analyte	Injected ($\mu\text{g/mL}$)	Intra-day			Inter-day		
		Found* (Conc. \pm SD)	Accuracy (R %)	Precision (RSD %)	Found* (Conc. \pm SD)	Accuracy (R %)	Precision (RSD %)
GSH	5.0	4.96 \pm 0.04	99.49	0.94	4.98 \pm 0.02	99.79	0.04
	17.0	17.02 \pm 0.14	99.23	0.85	16.89 \pm 0.11	99.39	0.71
	25.0	25.09 \pm 0.36	100.62	1.44	24.97 \pm 0.35	99.88	0.14

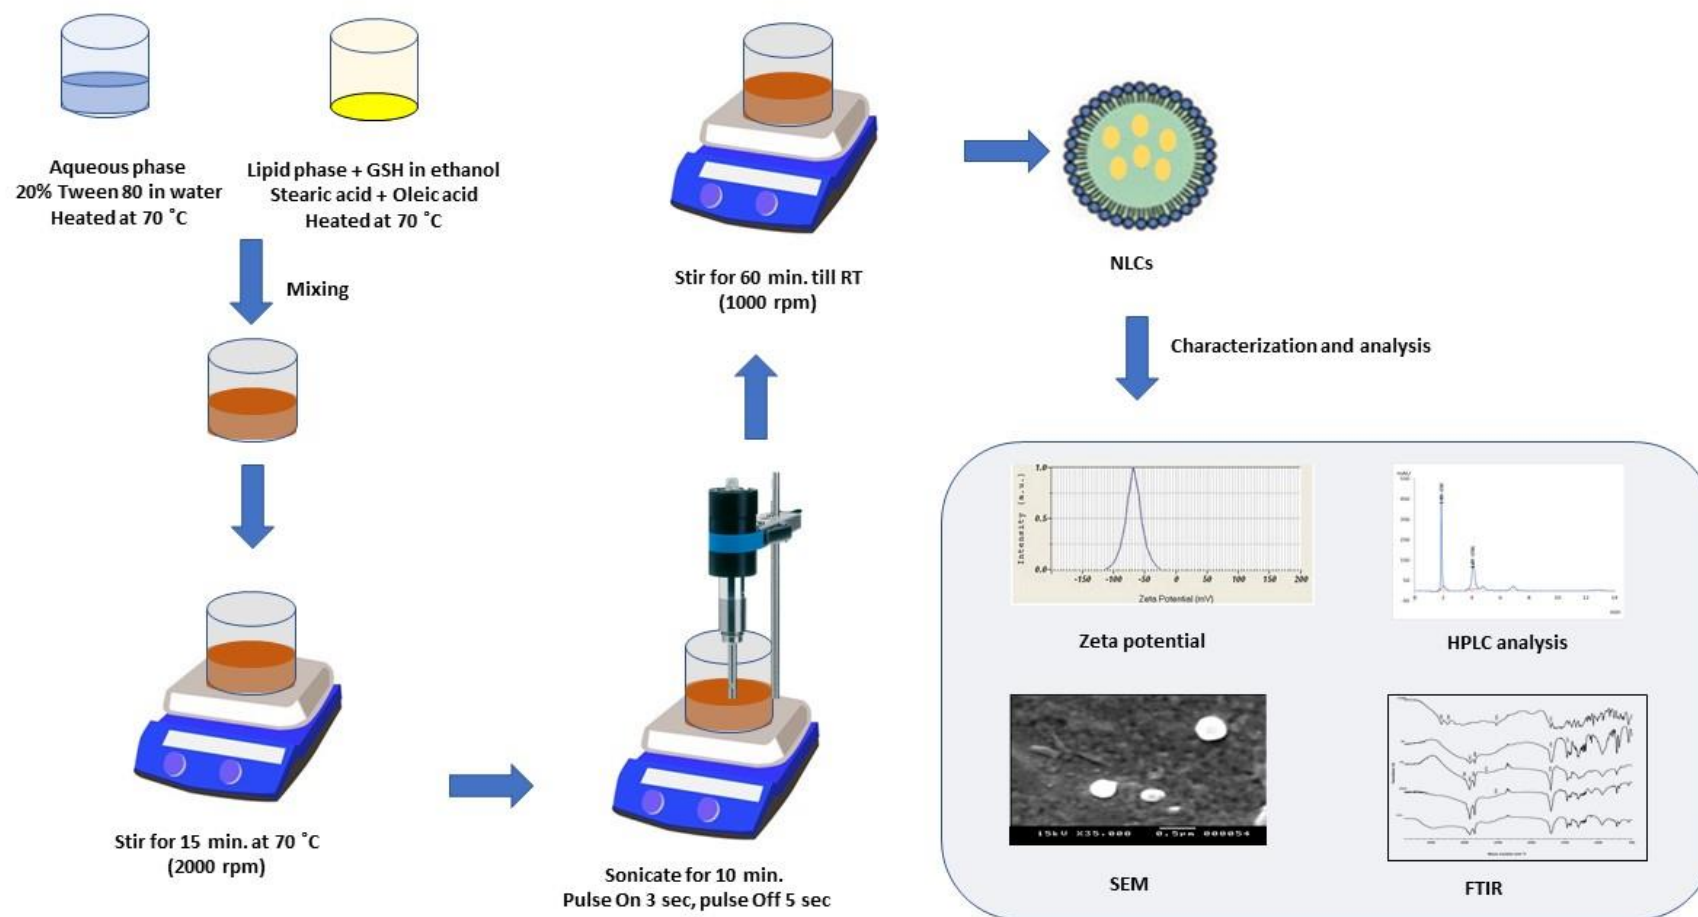


Figure S1: Scheme of GSH-NLCs preparation.