

Supplementary material

28-[1-(3-(Propionyloxy)propyl)-1H-1,2,3-triazol-4-yl]carbonylbetulin

Monika Kadela-Tomanek, Elwira Chrobak, Ewa Bębenek

Table of contents

Figure S1. ¹ H NMR spectrum (600 MHz, CDCl ₃) of 28-[1-(3-(propionyloxy)propyl)-1H-1,2,3-triazol-4-yl]carbonylbetulin.	2
Figure S2. ¹³ C NMR spectrum (150 MHz, CDCl ₃) of 28-[1-(3-(propionyloxy)propyl)-1H-1,2,3-triazol-4-yl]carbonylbetulin.	2
Figure S3. ESI-HRMS spectrum of 28-[1-(3-(Propionyloxy)propyl)-1H-1,2,3-triazol-4-yl]carbonylbetulin.....	3

Figure S1. ^1H NMR spectrum (600 MHz, CDCl_3) of 28-[1-(3-(propionyloxy)propyl)-1*H*-1,2,3-triazol-4-yl]carbonylbetulin.

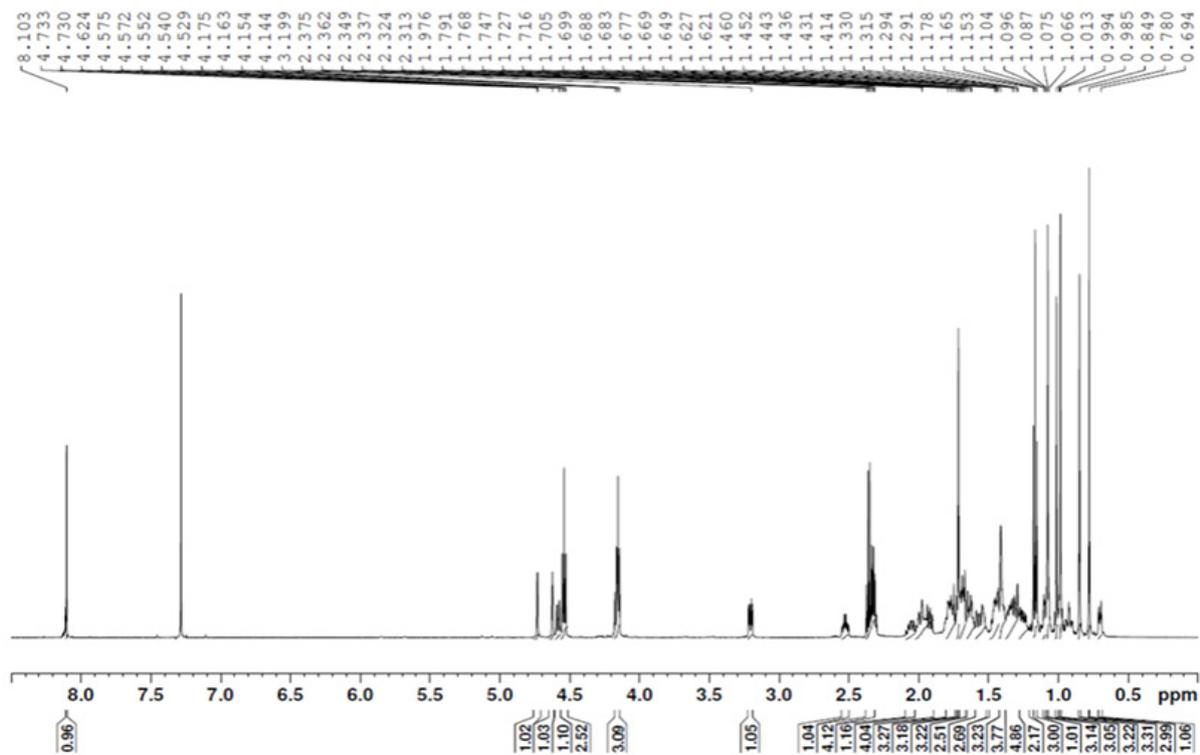


Figure S2. ^{13}C NMR spectrum (150 MHz, CDCl_3) of 28-[1-(3-(propionyloxy)propyl)-1*H*-1,2,3-triazol-4-yl]carbonylbetulin.


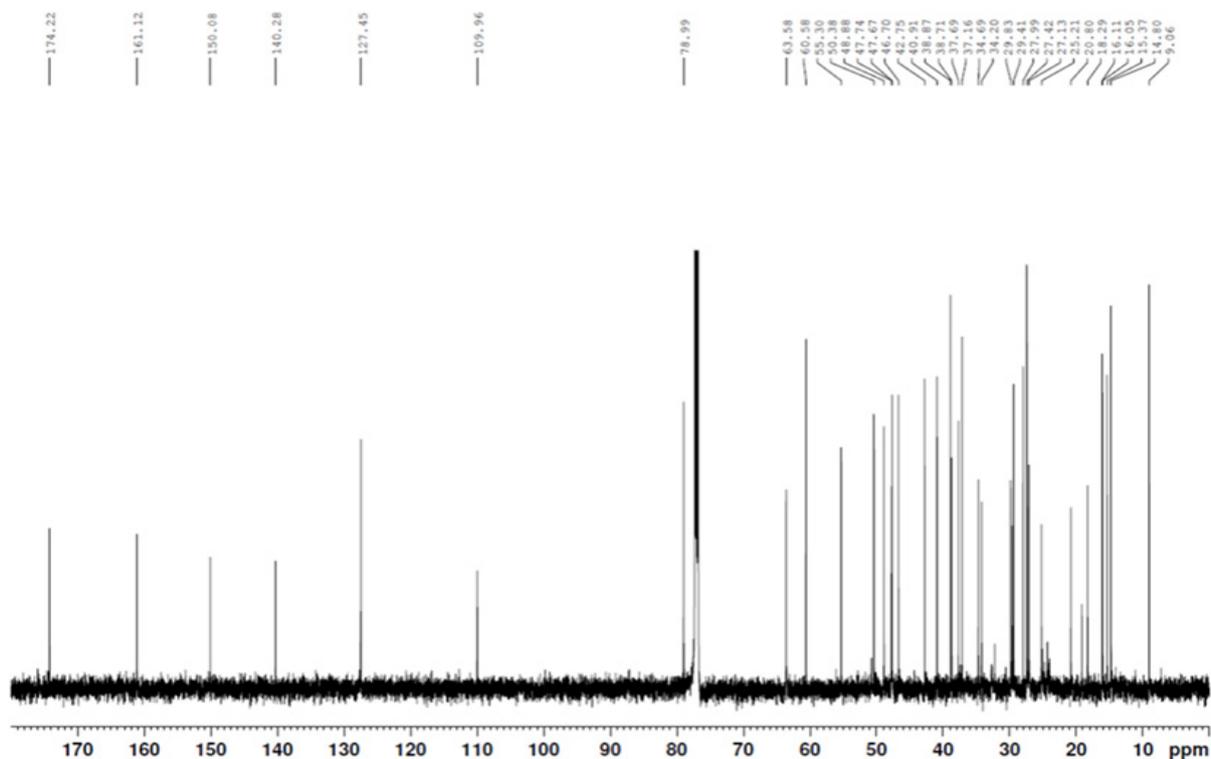



Figure S3. ESI-HRMS spectrum of 28-[1-(3-(Propionyloxy)propyl)-1H-1,2,3-triazol-4-yl]carbonylbetulin.

Compound Spectrum List Report					
Analysis Info			Acquisition Date 9/22/2022 1:16:45 PM		
Analysis Name	D:\Data\Service_20220831\MKT61.d		Operator	KM	
Method	low_mass.m		Instrument	impact II 1825265.10082	
Sample Name	tune_poshigh_test1		Comment		

Acquisition Parameter					
Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.3 Bar
Focus	Active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	300 m/z	Set End Plate Offset	-500 V	Set Dry Gas	3.0 l/min
Scan End	1000 m/z	Set Charging Voltage	2000 V	Set Divert Valve	Source
		Set Corona	0 nA	Set APCI Heater	0 °C

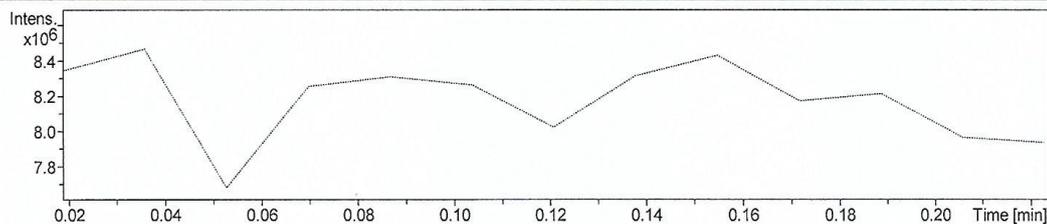

+MS, 0.0-0.2min #1-13

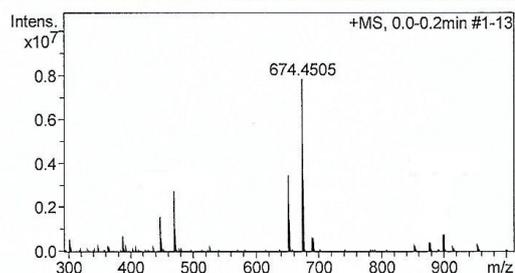

#	m/z	Res.	S/N	I	I %	FWHM
1	449.3852	34832	6147.2	1595371	20.5	0.0129
2	471.3669	38645	10455.1	2751086	35.3	0.0122
3	652.4687	43617	10201.4	3470885	44.5	0.0150
4	674.4505	48705	22184.9	7791122	100.0	0.0138