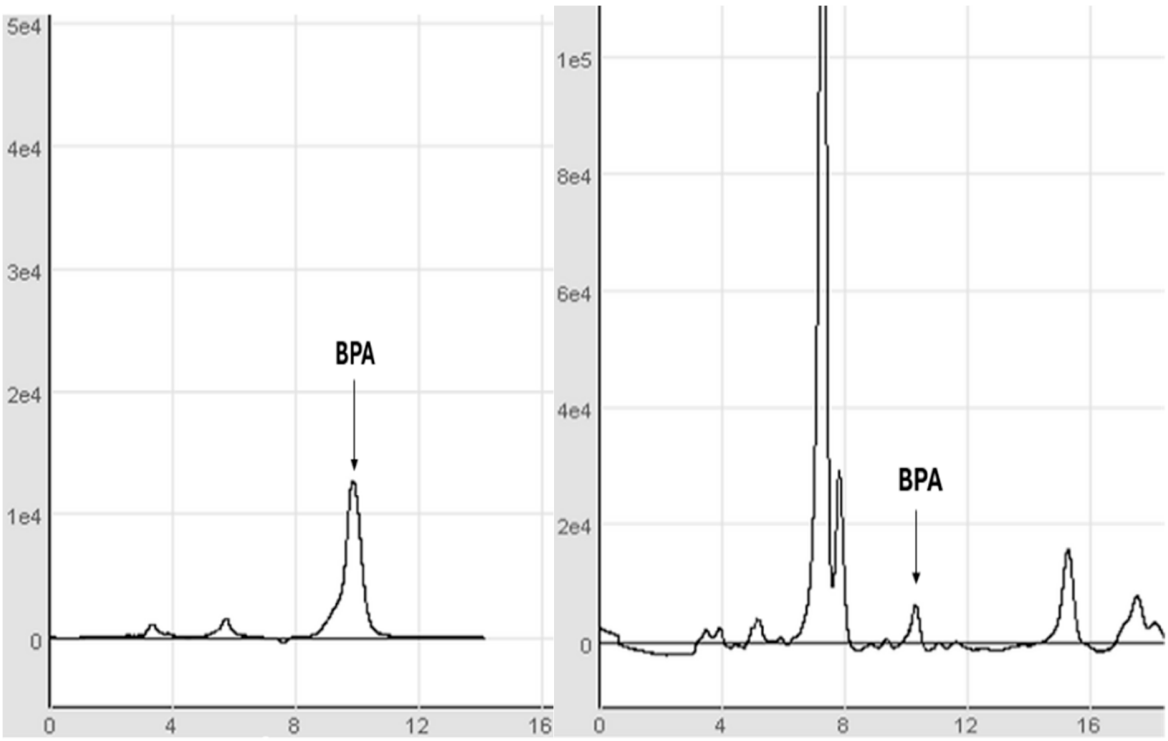


(a) (b)

Figure S1. (a) HPLC/FD chromatogram of the BPA standard (200 µg/L); (b) HPLC/FD chromatogram of a milk sample showing a positive detection of BPA.