


A

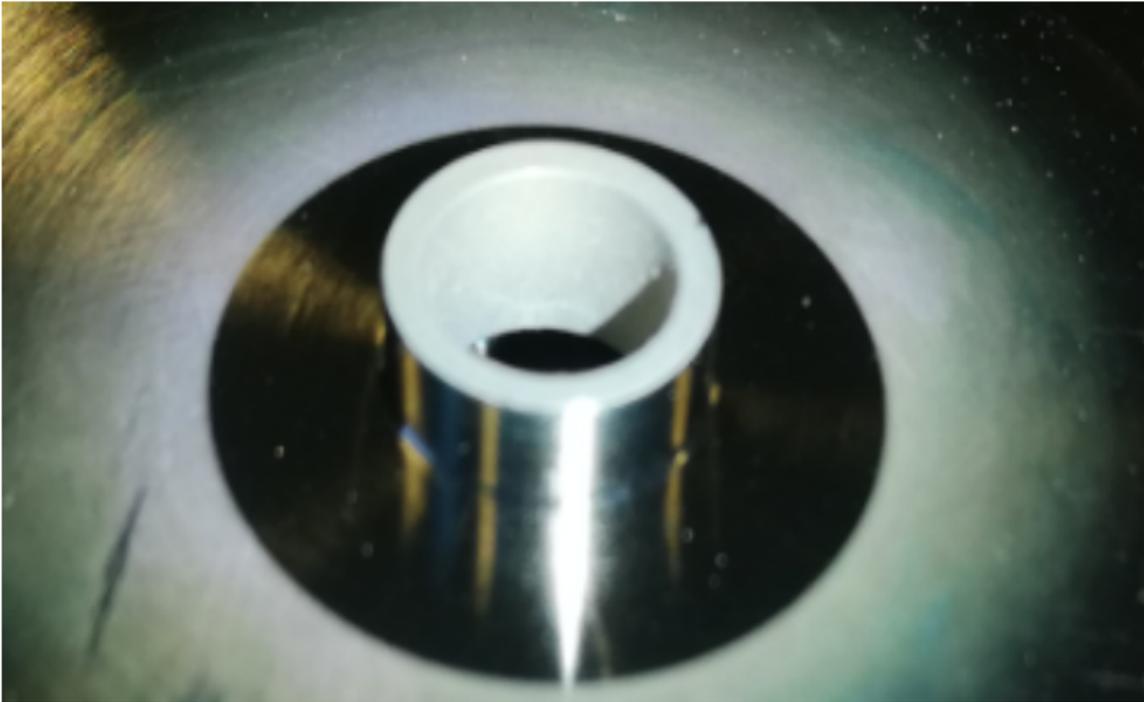

B

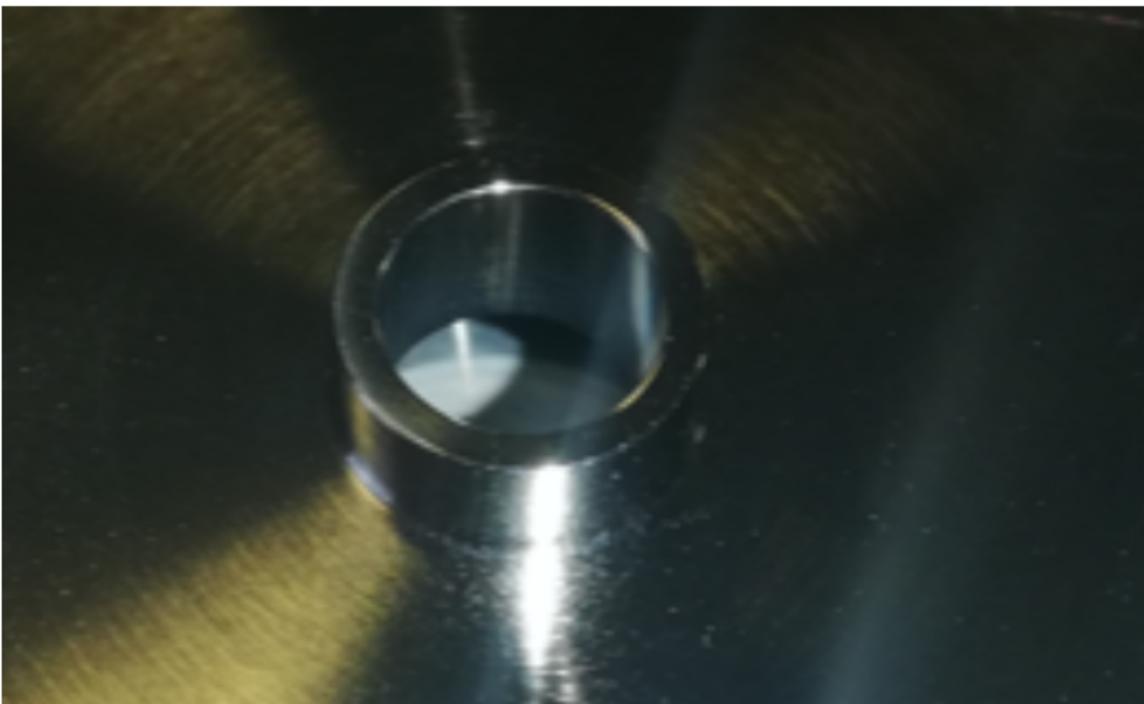


Figure S1. Fouling of primary lens from high throughput analysis of samples.