

Performance of Antigen Detection Tests for SARS-CoV-2: A Systematic Review and Meta-Analysis

Anastasia Tapari ^{1,†}, Georgia G. Braliou ^{1,†}, Maria Papaefthimiou ¹, Helen Mavriki ¹, Panagiota I. Kontou ¹, Georgios K. Nikolopoulos ² and Pantelis G. Bagos ^{1,*}

¹ Department of Computer Science and Biomedical Informatics, University of Thessaly, 35131 Lamia, Greece; atapari@dib.uth.gr (A.T.); gbraliou@dib.uth.gr (G.G.B.); mapapaef@gmail.com (M.P.); elenimavriki98@gmail.com (H.M.); pkontou@dib.uth.gr (P.I.K.)

² Medical School, University of Cyprus, Nicosia 1678, Cyprus; gknikolopoulos@gmail.com

* Correspondence: pbagos@compgen.org

† These authors contributed equally to this work.

Abstract: Coronavirus disease 2019 (COVID-19) initiated global health care challenges such as the necessity for new diagnostic tests. Diagnosis by real-time PCR remains the gold-standard method, yet economical and technical issues prohibit its use in points of care (POC) or for repetitive tests in populations. A lot of effort has been exerted in developing, using, and validating antigen-based tests (ATs). Since individual studies focus on few methodological aspects of ATs, a comparison of different tests is needed. Herein, we perform a systematic review and meta-analysis of data from articles in PubMed, medRxiv and bioRxiv. The bivariate method for meta-analysis of diagnostic tests pooling sensitivities and specificities was used. Most of the AT types for SARS-CoV-2 were lateral flow immunoassays (LFIA), fluorescence immunoassays (FIA), and chemiluminescence enzyme immunoassays (CLEIA). We identified 235 articles containing data from 220,049 individuals. All ATs using nasopharyngeal samples show better performance than those with throat saliva (72% compared to 40%). Moreover, the rapid methods LFIA and FIA show about 10% lower sensitivity compared to the laboratory-based CLEIA method (72% compared to 82%). In addition, rapid ATs show higher sensitivity in symptomatic patients compared to asymptomatic patients, suggesting that viral load is a crucial parameter for ATs performed in POCs. Finally, all methods perform with very high specificity, reaching around 99%. LFIA tests, though with moderate sensitivity, appear as the most attractive method for use in POCs and for performing seroprevalence studies.

Keywords: COVID-19; SARS-CoV-2; antigen test; meta-analysis; diagnostic performance; sensitivity; specificity

Citation: Tapari, A.; Braliou, G.G.; Papaefthimiou, M.; Mavriki, H.; Kontou, P.I.; Nikolopoulos, G.K.; Bagos, P.G. Performance of Antigen Detection Tests for SARS-CoV-2: A Systematic Review and Meta-Analysis. *Diagnostics* **2022**, *12*, 1388. <https://doi.org/10.3390/diagnostics12061388>

Academic Editor: Anna Baraniak

Received: 13 April 2022

Accepted: 24 May 2022

Published: 4 June 2022

Publisher's Note: MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Copyright: © 2022 by the authors. Licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

1. Introduction

COVID-19, caused by SARS-CoV-2, remains a global public health threat that has already claimed more than six million lives (<https://covid19.who.int>), with modeling estimates suggesting that this figure is probably much higher [1,2]. Vaccines, however, seem to perform well, especially after the administration of booster doses, providing moderate but short-lived protection from SARS-CoV-2 infection but significantly reducing COVID-19-related morbidity and mortality [3–9]. Non-pharmaceutical interventions (test-trace-isolate, hand washing, physical distancing, travel restrictions, school closures, closures of businesses, and stay-at-home orders) have also proved their effectiveness in containing the spread of the pandemic virus before the advent of vaccines [10–12]. Some of these measures will still be needed in our gradual efforts to return to normalcy. Testing in particular is essential to diagnosis, but also to developing and sustaining a reliable surveillance system for the years to come [13,14].

Real-time reverse transcription polymerase-chain-reaction (rt-PCR) test is the benchmark method for the clinical diagnosis of COVID-19 [15–17]. As such, it is designed for use with symptomatic people and has high analytical sensitivity. However, rt-PCR can detect viral genetic material even when the virus does not grow in a cell culture, suggesting that the presence of viral nucleic acid may not always reflect contagiousness. Moreover, it requires advanced laboratory equipment, specialist human resources, and significant infrastructure, often in a centralized setting, which increase costs, though these are less relevant for a single patient who needs a definite answer when he/she is tested. In summary, molecular diagnostic testing (nucleic acid amplification tests) becomes a less appealing method for frequent population screening to detect asymptomatic people with SARS-CoV-2 infection and as a tool to rapidly identify, contact-trace, and isolate highly infectious individuals. Antigen detection tests (AT) are immunoassays performed on pharyngeal, nasopharyngeal, nasal or throat swab specimens that detect the presence of a specific viral protein, which indicates viral activity [18,19]. The currently authorized AT include laboratory-based but also point-of-care (POC tests) and self-tests. AT are less expensive than rt-PCR, and most of them give results in approximately 15–30 min. In terms of weaknesses, AT are generally less sensitive than nucleic acid amplification tests. There are three main categories of AT used for the detection of SARS-CoV-2 infection. Lateral flow immunoassays (LFIA) are small, chromatography-based platforms used in POC. The sample is placed on the slot of the test plastic vector and an optical result (color) is obtained within 5–15 min [20]. Fluorescent immunoassays (FIA) are also small, handy, immunochromatography-based tests. The result is read by a fluorescence immunoassay analyzer within 5–20 min and can be performed in POC [21]. The chemiluminescence enzyme immunoassay (CLEIA) is a quick (about 30 min) and sensitive method to detect SARS-CoV-2 antigens. When the sample antigen reacts with the chemiluminescence substrate (antibody), the reaction product emits a photon of light instead of color development, which is read by an automated chemiluminescence analyzer [20].

Healthcare professionals, laboratory staff, and public health experts should comprehend the performance characteristics of AT, identify determinants of the accuracy of AT, and understand the differences among the three approaches to COVID-19-related testing (diagnostic, screening, and surveillance testing). In this respect, the aim of this meta-analysis is to comprehensively search the literature, to identify all relevant studies, to synthesize individual study estimates, and to determine the overall sensitivity and specificity of antigen-based methods for the detection of SARS-CoV-2, in comparison to quantitative rt-PCR (qPCR), for different types of clinical samples, and among both asymptomatic and symptomatic individuals.

2. Material and Methods

2.1. Literature Search Strategy

We conducted this systematic review and meta-analysis following the Preferred Reporting Items for Systematic Reviews and Meta-Analyses (PRISMA) guidelines [22] along with the advice for best practices [23]. We performed the literature search in Pubmed (<https://pubmed.ncbi.nlm.nih.gov> accessed on 15 May 2022), medRxiv (<https://www.medrxiv.org> accessed on 15 May 2022) and BioRxiv (<https://www.biorxiv.org>) up until 4 July 2021. The search terms were “(SARS-CoV-2 OR “Coronavirus disease 2019” OR COVID-19) AND antigen”. References from the selected studies were also scrutinized. Four independent researchers (AT, MP, HM, GB) evaluated search results; potential disagreements were resolved by discussion with GB and PB and consensus. Articles of all languages were considered to avoid gray literature publication bias [24].

2.2. Study Selection Criteria

Eligible criteria for inclusion in the meta-analysis were: (a) diagnosis of SARS-CoV-2 infection based on detection/quantitation of the viral genome by qPCR, according to World Health Organization (WHO)-, Centers for Disease Control (CDC)-, and European Centre for Disease Prevention and Control (ECDC)-approved methods [16,25–27]; (b) detection or measurement of nucleocapsid (N) or spike (S) proteins of SARS-CoV-2 (qualitatively or quantitatively depending on the method used); and (c) providing the necessary data that allow the calculation of sensitivity and specificity. We included studies that reported data on cases (positive samples) and healthy controls (negative samples) as well as studies with data available only for cases (see also Section 2.5).

2.3. Data Extraction

Data extraction was performed in a predetermined Microsoft Excel® sheet. From each study we extracted the following information: first author's last name, type of antigen used, type of sample, method of detection used, and the qPCR cycle threshold (Ct) values used for the detection of SARS-CoV-2 RNA. Additionally, the method of antigen testing used was recorded along with the brand name and the name of the manufacturer and the existence of data from the virus culture. Symptomatic and asymptomatic cases as well as male/female ratios were also recorded, if given. To obtain sensitivity and specificity measures, a 2×2 contingency table was constructed; thus, true positive (TP), false negative (FN), true negative (TN), and false positive (FP) results were recorded. In cases where no controls were used, we used TP and FN values only.

2.4. Study Outcomes

The primary outcome of this meta-analysis was the sensitivity and specificity of AT in relation to qPCR. Secondary outcomes included the performance of AT on different sample types (namely, nasopharyngeal, saliva, and throat samples) and by symptoms (asymptomatic versus symptomatic SARS-CoV-2 infected persons). We also explored the performance of AT across the number of qPCR Ct values (a higher Ct indicated lower viral load).

2.5. Data Analysis

The Quality Assessment of Diagnostic Accuracy Studies 2 (QUADAS-2 tool) was used to assess the quality of the included studies in terms of diagnostic accuracy [28]. The four domains assessed were patient selection, index test, reference standard, and flow and timing. Each domain was evaluated following classifications according to judgment, i.e., low risk, high risk, and unclear risk.

The bivariate meta-analytic method modified for the meta-analysis of diagnostic tests was used [29]. This method has been reported to be equivalent to the so-called hsROC method [30]. It uses logit-transforms of true positive rate (TPR) and false positive rate (FPR) in order to model sensitivity and specificity; it can also be used for the evaluation of between-studies variability (heterogeneity). Studies that include information only for logit (TPR)—that is, only for sensitivity—were included in the bivariate model under the missing at random (MAR) assumption in order to maximize statistical power and allow the modeling of between-studies variability and correlation [31]. Begg's rank correlation test [32] and Egger's regression test [33] were used on logit (TPR) to evaluate the presence of publication bias. Stata13 [34] was used to perform the analysis and run the command "mvmeta" with the method of moments for multivariate meta-analyses and meta-regression [35]. Statistical significance was set at $p < 0.05$; meta-analysis was performed when two or more studies were available, whereas tests for publication bias and meta-regression were performed when five or more studies were available.

3. Results

3.1. Characteristics of Studies

Following the literature search in Pubmed, MedRxiv, and BioRxiv by 4 July 2021, we retrieved 4700 unique articles (Figure 1). After scrutinizing abstracts and full papers and testing for eligibility criteria, we ended up with 235 articles, which included 31,387 SARS-CoV-2 infected individuals and 188,636 individuals without SARS-CoV-2 infection (total: 220,049 individuals). Two hundred and sixteen studies provided data on both cases and controls, while 19 studies reported results only for people with SARS-CoV-2 infection (Figure 1). Table 1 shows the characteristics of the included studies. All studies reported that SARS-CoV-2 infection was confirmed with qPCR of envelope (E), S or N protein according to WHO, CDC and ECDC guidelines. Various methods were used to identify or measure an antigen of SARS-CoV-2. The N antigen was investigated in 225 studies, the S antigen was investigated in eight studies, and in two studies, cumulative estimates were given for N + S or S + E + M (membrane) antigens. Four articles evaluated both N- and S-based assays. Most studies focused on rapid POC tests such as LFIA (181 studies), or FIA (38 studies). Chemiluminescence was used in 21 studies. In total, 83 different kits from 74 manufacturers and 18 in-house tests (LFIA, FIA, CLEIA) from the respective laboratories were used. Thirty-six studies used the same samples to compare different tests from different companies. Twelve studies used twelve unique techniques that are under development (LC-mass spectrometry [36,37], field-effect transistor (FET) based biosensing devices [38], organic electrochemical transistors-OECT [39], voltametric-based immunosensor [40], optical waveguide-based biosensor technology [41], deep learning-based surface-enhanced Raman spectroscopy [42], paper-based impedance sensor [43], high-field asymmetric waveform ion mobility spectrometry (FAIMS)-parallel reaction monitoring (PRM) [44], a colorimetric biosensor [45], an electrochemical glucose sensor [46], and a urine foaming test [47]). Finally, two studies were performed with urine samples [36,47]. Most studies used nasopharyngeal, nasal, pharyngeal, throat, oropharyngeal or saliva samples. We classified the samples into two groups, named “NSP”, containing the first three sample types, and “TS”, containing the last three types. The type of sample was clearly mentioned in 207 studies, while all types of samples were used without distinction in 31 studies. The results from different types of samples were compared with the same method in 11 studies. Finally, data from 60 studies on asymptomatic persons and 73 on symptomatic patients were also used to explore differences in diagnostic accuracy between these two patients’ groups. The results of the quality assessment of the research using the QUADAS tool are provided in Supplementary Table S1 and in Supplementary File S1.

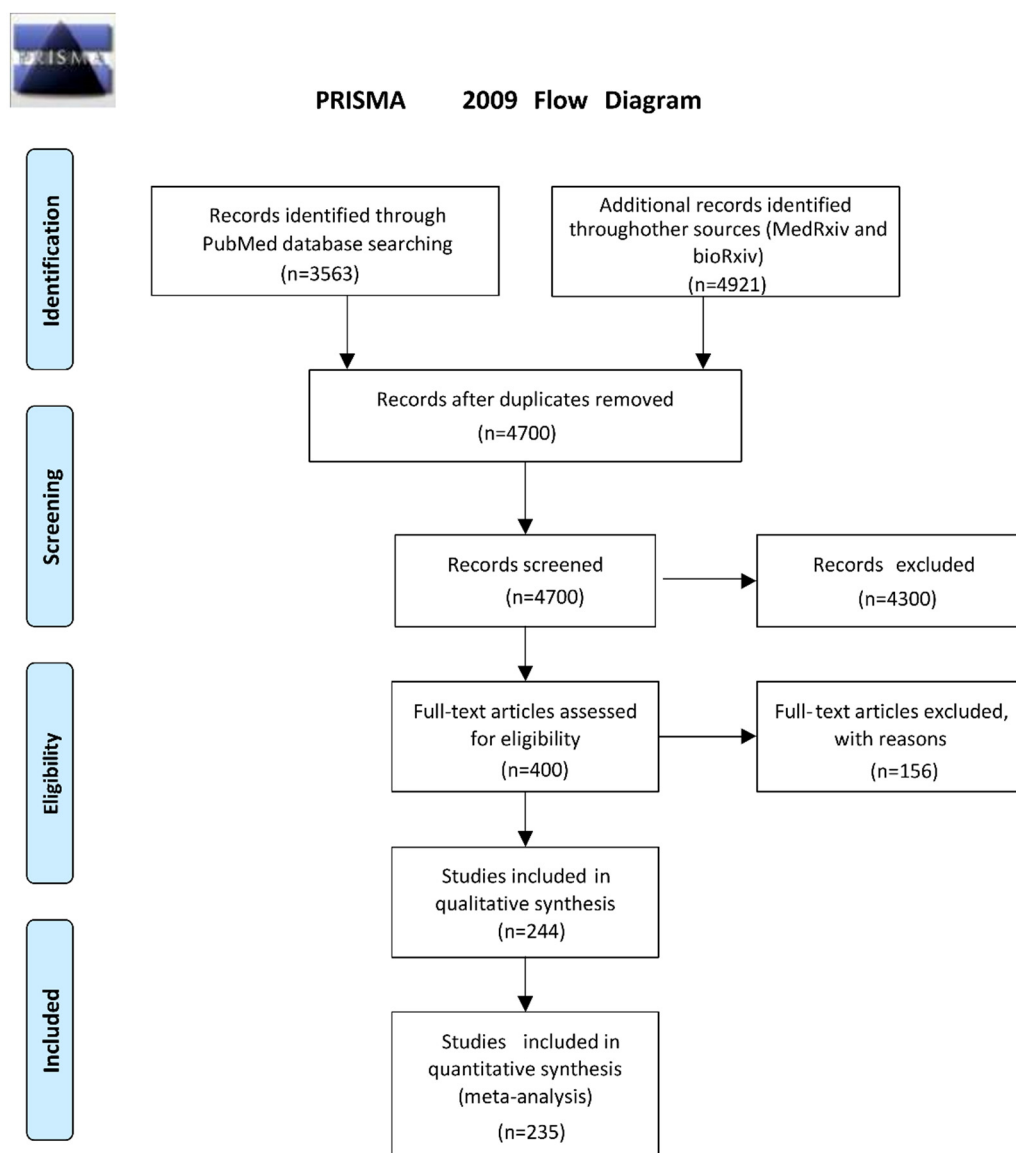


Figure 1. Preferred Reporting Items for Systematic Reviews and Meta-Analyses (PRISMA) flow diagram.

Table 1. Characteristics of the 235 studies included in the meta-analysis.

Author	Country of Study	Ag	Type of Sample	Ag Detection Method/Virus Culture Data	Kit Name	Kit Company	Ct Values Tested	Signal Detection [Rapid (w/wo Detector)/Quick]	Total Individuals	Cases	Controls
Mak et al. [48]	China	N	1. nsp 2. ts	1. LFIA 2. LFIA 3. LFIA/virus culture data	1. COVID-19 Ag Respi-Strip 2. NADAL COVID-19 Ag Test 3. Standard Q COVID-19 Ag	1. Coris Bioconcept, Belgium 2. Nal Von Minden GmbH, Germany 3. SD Biosensor, Korea	up to 20/up to 30/up to 40/0–20/20–30/30–40	Rapid	35	35	NA
Linares et al. [49]	Spain	N	nsp	LFIA	Panbio COVID-19 Ag Rapid Test Device	Abbott Rapid Diagnostic Jena GmbH, Jena, Germany	Up to 40	Rapid	255	60	NA
Gupta et al. [50]	India	N	nsp	LFIA	Standard Q rapid antigen detection test	SD Biosensor, Inc., Gurugram	Up to 40	Rapid	330	77	253
Fenollar et al. [51]	France	N	nsp	LFIA	PANBIO COVID -19 Ag rapid test device	Abbott, USA	Up to 40	Rapid	341	204	137
Nalumansi et al. [52]	Uganda	N	nsp	LFIA	STANDARD Q COVID-19 Ag Test	SD -Biosensor, Republic of Korea	Up to 30/up to 40/30–40	Rapid	262	90	172
Parada-Ricart et al. [53]	Spain	N	nsp	FIA	2019-nCoV Antigen Rapid Test Kit (FIA)	Shenzhen Bioeasy Biotechnology CO LTD, China	Up to 40	Rapid/detector	172	26	146
Lee et al. [54]	Korea	S	nsp	LFIA/virus culture data	In-house test		Up to 40	Rapid/detector	8	3	5
Cerutti et al. [55]	Italy	N	nsp	LFIA	STANDARD Q COVID19 Ag	SD-Biosensor, RE-LAB, I	Up to 40	Rapid	330	109	221
Diao et al. [56]	China	N	nsp	FIA	In-house test		Up to 40	Rapid/detector	502	356	146
Young et al. [57]	USA	N	nsp	1. LFIA 2. FIA	1. BD Veritor™ System 2. Sofia 2 SARS Antigen FIA	1. Becton-Dickinson and Company, USA 2. Quidel, San Diego, CA	Up to 40	1. Rapid/optional detector 2. Rapid/detector	612	81	531
Liotti et al. [58]	Italy	N	nsp	FIA	STANDARD F COVID19 Ag (FIA)	SD Biosensor, Suwon, Korea	Up to 20/up to 30/up to 40/0–20	Rapid/detector	359	104	255

Ogawa et al. [59]	Japan	N	Nsp	CLEIA	Lumipulse SARS-CoV-2 Ag	Fujirebio, Tokyo, Japan	Up to 40	Detector	325	24	301
Hirotsu et al. [60]	Japan	N	nsp	CLEIA	LUMIPULSE SARS-CoV-2 Ag kit	Fujirebio, Inc. (Tokyo, Japan)	Up to 40	Detector	313	58	255
Nagura-Ikeda et al. [61]	Japan	N	ts	LFIA	Espline SARS-CoV-2	Fuji Rebio Inc.	Up to 40	Rapid	103	84	19
Mak et al. [62]	Hong Kong	N	1. nsp/ts 2. ts	LFIA	BIOCREDIT COVID-19 Ag kit	RapiGEN Inc.	Up to 20/up to 30/up to 40/0–20/20–30	Rapid optional detector	160	51	109
Mertens et al. [63]	Belgium	N	nsp	LFIA/virus culture data	COVID-19 Ag RespiStrip	Coris BioConcept	Up to 30/up to 40	Rapid	328	132	196
Blairon et al. [64]	Belgium	N	nsp	LFIA	COVID-19 Ag RespiStrip	Coris Bioconcept, Gembloux, Belgium	Up to 40	Rapid	774	159	615
Porte et al. [21]	Chile	N	nsp/ts	FIA	2019-nCoV Antigen Rapid Test Kit (FIA)	Bioeasy Biotechnology Co., Shenzhen, China	Up to 30	Rapid/detector	127	82	45
Schohy et al. [65]	Belgium	N	nsp	LFIA	COVID-19 Ag RespiStrip	Coris BioConcept, Gembloux, Belgium	Up to 40	Rapid	148	106	62
Lambert-Niclot et al. [66]	France	N	nsp	LFIA	COVID-19 Ag RespiStrip	Coris BioConcept, Gembloux, Belgium	Up to 40	Rapid	138	94	44
Diao et al. [67]	China	N	nsp	FIA	In-house test		Up to 30/up to 40/30–40	Rapid	239	208	31
Beck et al. [68]	Milwaukee	N	nsp	FIA	Sofia SARS FIA test (SOFIA)	Quidel, San Diego, CA	Up to 40	Rapid/detector	346	61	285
Krüttgen et al. [69]	Germany	N	nsp	LFIA	SARS-CoV-2 Rapid Antigen Test	Roche, Switzerland	Up to 20/up to 30/up to 40/0–20/20–30/30–40	Rapid	150	75	75
Albert et al. [70]	Spain	N	nsp	LFIA/virus culture data	Panbio™ COVID-19 Ag Rapid Test Device	Abbott Diagnostic GmbH, Jena, Germany	Up to 40	Rapid	412	54	358
Chaimayo et al. [71]	Thailand	N	nsp/ts	LFIA	Standard Q COVID-19 Ag test	SD Biosensor®, Chuncheongbuk-do, Republic of Korea	Up to 40	Rapid	454	60	394

Lanser et al. [72]	Austria	N	nsp	LFIA	Panbio™ COVID-19 Ag Rapid test	Abbott, Chicago, Illinois	Up to 30/up to 40/30–40	Rapid	53	51	2
Gremmels et al. [73]	The Netherlands/Aru ba	N	nsp	LFIA	Panbio COVID-19 Ag rapid test device	Abbott, Lake Country, IL, USA	Up to 40	Rapid	2948	202	2746
Drevinek et al. [74]	Czech Republic	N	nsp	1. LFIA 2. FIA	1. Panbio COVID-19 Ag Rapid Test 2. Standard F COVID-19 Ag FIA	1. Abbott, Germany 2. SD Biosensor, Republic of Korea	Up to 20/up to 30/up to 40/0–20/20–30/30–40	1. Rapid 2. Rapid/detector	591	223	368
Schwob et al. [75]	Switzerland	N	nsp	1. LFIA 2. LFIA 3. LFIA	1. STANDARD Q COVID-19 Ag Test 2. Panbio COVID-19 Ag Test 3. COVID-VIRO	1. SD -Biosensor, Republik of Korea 2. Abbott, Germany 3. AAZ-LMB	Up to 40	Rapid	928	372	556
Corman et al. [76]	Germany	N	nsp	1. LFIA 2. LFIA 3. LFIA 4. LFIA 5. LFIA 6. LFIA 7. LFIA/virus culture data	1. Panbio COVID-19 Ag Test 2. BIOCREREDIT COVID-19 Ag kit 3. Coronavirus Ag Rapid Test Cassette (swab) 4. COVID-19 Ag Respi-Strip 5. RIDA®QUICK SARS-CoV-2 antigen 6. NADAL COVID19-Ag Test 7. SARS-CoV-2 Rapid Antigen Test	1. Abbott, Germany 2. RapiGEN Inc. 3. Healgen 4. Coris Bioconcept, Gembloux, Belgium 5. R-Biopharm 6. NAL von minden 7. Roche	Up to 40	Rapid	150	115	35
Abdulrahman et al. [77]	Bahrain	N	nsp	LFIA	Panbio COVID 19 antigen rapid test device	Abbott Rapid Diagnostic Jena GmbH, Jena, Germany	Up to 30	Rapid	4183	733	3450
Yokota et al. [78]	Japan	N	Nsp,ts	1. LFIA 2. CLEIA	1. Espline SARS-CoV-2	1. Fujirebio, Tokyo, Japan	Up to 30/up to 40/20–30	1. Rapid 2. Quick/detector	34	34	NA

					2. Lumipulse SARS-CoV-2 Ag kit	2. Fujirebio, Tokyo, Japan					
Nash et al. [79]	USA/Brazil	1. N 2. S	nsp	LFIA	In-house		Up to 20/up to 30/up to 40/0–20/20–30/30–40	Rapid	311	172	139
Van der Moeren et al. [80]	The Netherlands	N	nsp	LFIA	BD Veritor™ System	Becton-Dickinson and Company, USA	Up to 20/up to 30/up to 40/0–20/20–30	Rapid/optional detector	351	17	334
Porte et al. [81]	Chile	N	nsp/ts	1. FIA 2. FIA	1. SOFIA SARS Antigen FIA 2. STANDARD® F COVID-19 Ag FIA	1. Quidel Corporation, San Diego, CA, USA 2. SD Biosensor Inc., Gyeonggi-do, Republic of Korea	Up to 30/up to 40/30–40	Rapid/detector	91	59	32
Krüger et al. [82]	Germany/UK	N	nsp/ts	1. FIA 2. LFIA 3. LFIA/virus culture data	1. 2019-nCoV Ag Fluorescence Rapid Test Kit 2. COVID-19 Ag Respi-Strip 3. STANDARD Q COVID-19 Ag Test	1. Shenzhen Bioeasy Biotechnology Co. Ltd., Guangdong Province, China 2. Coris Bioconcept, Gembloux, Belgium 3. SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 30/up to 40/30–40	1. Rapid/detector 2. Rapid 3. Rapid	2407	72	2335
Singh et al. [46]	San Diego	S	nsp	ECGluS	In-house		Up to 40	Quick *	24	16	8
Ventura et al. [83]	Italy	S + E + M	Nsp/ts	CBS	In-house		Up to 40	Detector	94	45	49
Herrera et al. [84]	Florida	N	nsp	LFIA	NR/AdventHealth Centra Care		Up to 40	Rapid	1669	486	1183
Renuse et al. [44]	USA	N	nsp	FAIMS-PRM	In-house		Up to 40	Detector	176	88	88
Pickering et al. [85]	UK	N	nsp-ts	LFIA/virus culture data	1. Innova Rapid SARS-CoV-2 Antigen Test 2. Spring Healthcare SARS-CoV-2	1. Xiamen Biotime Biotechnology, Fujian, China 2. Shanghai ZJ Bio-Tech, Shanghai, China	20–30	Rapid	200	100	100

					Antigen Rapid Test Cassette	3. E25Bio, Cambridge, MA, USA					
					3. E25Bio Rapid Diagnostic Test	4. Zhuhai Encode Medical Engineering, Zhuhai, China					
					4. Encode SARS-CoV-2 Antigen Rapid Test Device	5. SureScreen Diagnostics, Derby, UK					
					5. SureScreen COVID-19 Rapid Antigen Test Cassette						
Harmon et al. [86]	Washington	N	nsp	FIA	Sofia-2 SARS-CoV-2 Antigen Tests	Quidel, San Diego, CA	Up to 40	Rapid/detector	23,462	83	23,379
Korenkov et al. [87]	Germany	N	nsp-ts	LFIA/virus culture data	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 20/up to 30/up to 40/0–20/20–30/30–40	Rapid	2028	210	1818
Ehsan et al. [43]	Saudi Arabia	S	nsp	Paper-based impedance sensor	In-house		Up to 40	Detector	5	3	2
Seynaeve et al. [88]	Belgium	N	nsp	LFIA	1. COVID-19 Ag Respi-Strip 2. coronavirus antigen rapid test cassette	1. Coris Bioconcept, Belgium 2. Healgen Scientific, LLC, USA	Up to 30/ Up to 40/30–40	Rapid	163	98	65
Di Domenico et al. [89]	Italy	1. N 2. S	1. nsp 2. ts	1. ELISA based 2. LFIA/virus culture data	1. Portable COVID-19 Antigen Lab Test 2. Panbio™ COVID-19 Ag Rapid Test Device	1. Stark 2. Abbott Diagnostic GmbH, Jena, Germany	Up to 40	Rapid	433	36	397
Kiro et al. [90]	India	N	nsp	FIA	STANDARD® F COVID-19 Ag FIA	SD Biosensor Inc., Gyeonggi-do, Republic of Korea	Up to 40	Rapid/detector	354	136	218
Smith et al. [91]	Illinois	N	1. nsp-ts 2. nsp	FIA/virus culture data	SOFIA SARS Antigen FIA	Quidel Corporation, San Diego, CA, USA	Up to 40	Rapid/detector	43	43	NA
L’Huillier et al. [92]	Switzerland	N	nsp	LFIA	Panbio™ COVID-19 Ag Rapid Test Device	Abbott Diagnostic GmbH, Jena, Germany	Up to 40	Rapid	822	119	703

Gupta et al. [93]	India	S	nsp	ELISA	In-house	Up to 40	Quick	232	44	188	
Wagenhäuser et al. [94]	Germany	N	ts	LFIA	1. NADAL COVID-19 Ag Test 2. Panbio COVID-19 Ag rapid test device 3. MEDsan SARS-Cov-2 Antigen Rapid Test	1. Nal Von Minden GmbH, Germany 2. Abbott Laboratories, Abbott Park IL, USA 3. MEDsan GmbH, Hamburg, Germany	Up to 40	Rapid	5056	101	4955
Fernandez et al. [95]	Spain	N	nsp	FIA	LumiraDx™	LumiraDx™ Limited, Londres, Reino Unido	Up to 40	Rapid/detector	46	24	22
Amer et al. [96]	Egypt	N	nsp-ts	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 40	Rapid	47	45	2
Baccani et al. [97]	Italy	N	nsp	1. CLEIA 2. FIA 3. FIA	1. Lumipulse G SARS-CoV-2 Ag 2. STANDARD® F COVID-19 Ag FIA 3. AFIAS COVID-19 Ag	1. Fujirebio, Tokio, Japan 2. SD Biosensor; Suwon-si, Korea 3. Menarini; Florence, Italy	Up to 30/Up to 40/30–40	1. Quick/detector 2. Rapid/detector 3. Rapid/detector	375	85	290
Matsuzaki et al. [98]	Japan	N	nsp	CLEIA	1. VITROS® SARS-CoV-2 Antigen Test 2. LUMIPULSE® SARS-CoV-2 Ag Test	2. Ortho Clinical Diagnostics, Rochester, NY, USA 3. Fujirebio, Tokio, Japan	Up to 40	1. Quick/detector 2. Quick/ detector	128	49	79
Jakobsen et al. [99]	Denmark	N	nsp	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 40	Rapid	4811	221	4590
Ngo Nsoga et al. [100]	Switzerland	N	nsp-ts	LFIA/virus culture data	Panbio™ COVID-19 Ag Rapid Test Device	Abbott Diagnostic GmbH, Jena, German	Up to 40	Rapid	402	168	234
Funabashi et al. [41]	Japan	N	nsp	Optical waveguide-based biosensor technology	In-house		Up to 40	Detector	64	34	30
Smith et al. [101]	Maryland	N	nsp	FIA	SOFIA SARS Antigen FIA	Quidel Corporation, San Diego, CA, USA	Up to 40	Rapid/detector	2887	235	2652

Eleftheriou et al. [102]	Greece	N	nsp	LFIA	Panbio™ COVID-19 Ag Rapid Test Device	Abbott Diagnostic GmbH, Jena, Germany	Up to 40	Rapid	744	51	693
Huang et al. [42]	China	S	ts	Deep learning-based surface-enhanced Raman spectroscopy	In-house		Up to 40	NA/detector	57	30	27
Lindner et al. [103]	Germany	N	nsp-ts	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	146	40	106
Ferte et al. [104]	France	N	nsp	LFIA	Panbio™ COVID-19 Ag Rapid Test Device	Abbott Diagnostic GmbH, Jena, Germany	Up to 40	Rapid	688	52	636
Fernandez-Montero et al. [105]	Spain	N	nsp-ts	LFIA	SARS-CoV-2 Rapid Antigen Test	Roche	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	2543	49	2494
Hoehl et al. [106]	Germany	N	nsp	LFIA	RIDA®QUICK SARS-CoV-2 Antigen	R-Biopharm AG	Up to 30	Rapid	9	9	NA
Lee et al. [107]	Korea	N	nsp	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	680	380	300
Mayanskiy et al. [108]	Russia	N	nsp	ELISA	CoviNag EIA	XEMA, Russia	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Detector	277	182	95
Leixner et al. [109]	Austria	N	nsp	LFIA	AMP Rapid Test SARS-CoV-2 Ag	AMP Diagnostics, AMEDA Labordiagnostik GmbH, Graz, Austria	Up to 30/Up to 40/30–40	Rapid	392	94	298
Hirotsu et al. [110]	Japan	N	nsp	1. CLEIA 2. CLEIA	1. LUMIPULSE® SARS-CoV-2 Ag Test 2. Elecsys1 SARS-CoV-2 Antigen Assay	1. Fujirebio, Tokyo, Japan 2. Roche, Basel, Switzerland	Up to 40	Detector	637	487	150
Chavan et al. [36]	USA	N	urine	mass spectrometry	In-house		Up to 40	Detector	50	39	11
Fiedler et al. [111]	Germany	N	nsp	CLEIA/virus culture data	LIAISON® SARS-CoV-2 Ag	DiaSorin	Up to 40	Detector	182	110	72

Dierks et al. [112]	Germany	N	nsp	1. FIA 2. LFIA	1. LumiraDx™ 2. NADAL COVID-19 Ag Test	1. LumiraDx™ Limited, London, United Kingdom 2. Nal Von Minden GmbH, Germany	Up to 40	1. Rapid/detector 2. Rapid	444	11	433
Terpos et al. [113]	Slovenia	N	nsp	LFIA	COVID-19 Antigen Detection Kit (Colloidal Gold)	Zhuhai Lituo Biotechnology Co., Ltd.	Up to 30/Up to 40/30–40	Rapid	358	114	244
Osmanodja et al. [114]	Germany	N	nsp-ts	LFIA	Dräger Antigen Test SARS-CoV-2	Dräger Safety AG and Co. KGaA, Lübeck, Germany	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	379	70	309
Harris et al. [115]	USA	N	nsp	FIA	SOFIA SARS Antigen FIA	Quidel Corporation, San Diego, CA, USA	Up to 30/Up to 40/30–40	Rapid/detector	2429	324	2105
Cento et al. [116]	Italy	N	nsp	FIA	LumiraDx™	LumiraDx™ Limited, Londres, Reino Unido	Up to 30/Up to 40/30–40	Rapid/detector	960	347	613
Kumar et al. [117]	India	N	nsp	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 40	Rapid	6	6	NA
Orsi et al. [118]	Italy	N	nsp	FIA	1. FREND™ COVID-19 Ag 2. STANDARD® F COVID-19 Ag FIA	1. NanoEntek, Korea 2. SD Biosensor; Suwon-si, Korea	Up to 30/Up to 40/30–40	Rapid/detector	110	60	50
Blairon et al. [119]	Belgium	N	nsp	LFIA/virus culture data	1. Coronavirus Ag Rapid Test Cassette 2. GSD NovaGen SARS-CoV-2 (COVID-19) Antigen Rapid Test 3. Aegle Coronavirus Ag Rapid Test Cassette	1. BioRad 2. NovaTec Immunodiagnostica GmbH 3. LumiraDx	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	199	97	102
Bornemann et al. [120]	Germany	N	nsp	FIA	SOFIA SARS Antigen FIA	Quidel Corporation, San Diego, CA, USA	Up to 30/Up to 40/30–40	Rapid/detector	1391	91	1300
Kruger et al. [121]	Germany	N	1. nsp 2. ts 3. nsp-ts	LFIA	Panbio™ COVID-19 Ag Rapid Test Device	Abbott Diagnostic GmbH, Jena, Germany	Up to 30/Up to 40/30–40	Rapid	1108	106	1002

Eissa et al. [40]	Saudi Arabia	N	nsp	Voltammetric-based immunosensor	In-house		Up to 30/Up to 40/30–40	Detector	6	5	1
Shaikh et al. [122]	USA	N	nsp	LFIA	BinaxNOW™ COVID-19 Ag Card	Abbott Diagnostics Scarborough, Inc., USA	Up to 40	Rapid	199	39	160
Diez Flecha et al. [123]	Spain	N	nsp	LFIA	Panbio™ COVID-19 Ag Rapid Test Device	Abbott Diagnostic GmbH, Jena, Germany	Up to 30/Up to 40/30–40	Rapid	55	49	6
Yokota et al. [124]	Japan	N	ts	CLEIA	In-house		Up to 40	detector	2056	89	1967
Guo et al. [39]	Saudi Arabia	N	1. nsp 2. ts 3. nsp-ts	OECT	In-house		Up to 40	detector	24	11	13
Klein et al. [125]	Germany	N	nsp	LFIA	Panbio™ Ag-RDT	Abbott Diagnostics, Jena, Germany	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	290	39	251
Caramello et al. [126]	Italy	N	nsp	1. LFIA 2. FIA	1. SD BIOSENSOR Ag-RDT 2. LUMIRADX Ag-RDT	1. SD BIOSENSOR Ag-RDT 2. LumiraDx UK Ltd., Dumyat Business Park, Alloa, FK10 2PB, UK)	Up to 40	1. Rapid 2. Rapid/detector	324	210	114
Koeleman et al. [127]	Netherlands	N	nsp-ts	LFIA	1. Certest SARS-CoV-2 2. Roche SARS-CoV-2 Rapid Antigen Test 3. Romed Coronavirus Ag Rapid Test 4. BD Veritor SARS-CoV-2 point-of-care test 5. Panbio™ COVID-19 Antigen rapid test	1. Certest Biotec S.L., Spain 2. Roche, Switzerland 3. Romed, The Netherlands 4. Becton, Dickinson and Company, USA 5. Abbott, USA	Up to 40	Rapid	980	340	640
Šterbenc et al. [128]	Slovenia	N	nsp	LFIA	SARS-CoV-2 rapid antigen test (Roche)	Roche Diagnostics GmbH, Mannheim, Germany)	Up to 40	Rapid	191	2	189

Kumar et al. [129]	India	N	nsp-ts	FIA	STANDARD™ Q COVID-19 Ag test kit	SD Biosensor; Suwon-si, Korea	Up to 40	Rapid/detector	204	12	192
Soleimani et al. [130]	Belgium	N	nsp	FIA	1. COVID19Speed- antigen test 2. Panbio™ COVID- 19 Ag rapid test	1. BioSpeedia 2. Abbott	Up to 30/Up to 40/30–40	Rapid/detector	401	196	205
Takeuchi et al. [131]	Japan	N	nsp	LFIA	QuickNavi- COVID19 Ag	Denka Co., Ltd., To- kyo, Japan	Up to 30	Rapid	862	51	811
Linares et al. [49]	Spain	N	nsp	1. LFIA 2. FIA	1. Panbio COVID-19 Ag Rapid Test De- vice 2. D-Biosensor STANDARD F COVID-19 Ag	1. Abbot Rapid Diag- nostics GmbH, Jena 2. SD Biosensor, Inc.	Up to 20/Up to 30/20–30	1. Rapid 2. Rapid/detector	356	170	186
Homza et al. [132]	Czech Re- public	N	nsp	LFIA	Ecotest COVID-19 Antigen Rapid Test	Assure Tech, Hang- zhou, China	Up to 20/Up to 30/Up to 40/0– 20/20–30/30–40	Rapid	491	164	327
Van der Moeren et al. [133]	Nether- lands	N	nsp-ts	CLEIA	BD veritor system for rapid detection of SARS-CoV-2 (VRD)	Becton-Dickinson and Company, USA	20–30	Detector	978	161	817
Brihn et al. [134]	USA	N	nsp	FIA	Quidel Sofia 2 SARS Antigen Fluorescent Immunoassay	Quidel Corporation	Up to 30	Rapid/detector	2039	149	1890
Nordgren et al. [135]	Sweden	N	nsp	LFIA/virus culture data	1. Panbio™ COVID- 19 Ag Rapid Test 2. Zhejiang Orient Gene	1. Abbott 2. Healgen Biotech Coronavirus Ag rapid test cassette	Up to 20/Up to 40/20–30	Rapid	462	156	306
Holzner et al. [136]	Germany	N	nsp	LFIA	Standard Q COVID- 19 Ag	SD Biosensor, Korea	Up to 30	Rapid	2280	456	1824
Kim et al. [137]	Korea	N	nsp	LFIA	GenBody COVID-19 Ag Test (CO- VAG025)	GenBody Inc.	Up to 40/20–30	Rapid	330	130	200
Bianco et al. [138]	Italy	N	nsp	FIA	LumiraDx™ SARS- CoV-2 Antigen Test	LumiraDx	30–40	Rapid/detector	907	298	609
Peña et al.	Chile	N	nsp	LFIA	SARS-CoV-2 RAT	SD Biosensor	Up to 30	Rapid	842	73	769

[139]												
Muhi et al. [140]	Australia	N	nsp	LFIA/virus culture data	PanBioTM COVID-19 Ag	Abbott	Up to 40	Rapid	189	26	163	
Uwamino et al. [141]	Japan	N	nsp	LFIA/virus culture data	Espline SARS-CoV-2 RAD	FUJIREBIO, Tokyo, Japan	Up to 40	Rapid	117	25	92	
Thakur et al. [142]	India	N	nsp-ts	LFIA	PathoCatch	ACCUCARE	20–30	Rapid	677	84	593	
Homza et al. [143]	Czech Republic	N	nsp	LFIA/virus culture data	1. SARS-CoV-2 Antigen Rapid Test Kit 2. Ecotest COVID-19 Antigen Rapid Test 3. Standard Q COVID-19 Ag 4. Immupass VivaDiag™ SARS-CoV-2 Ag Rapid Test 5. ND COVID-19 Ag test	1. JOYSBIO (Tianjin) Biotechnology Co., Ltd., Tianjin, China 2. Assure Tech, Hangzhou, China 3. SD Biosensor, Korea 4. VivaChek Biotech (Hangzhou) Co., Ltd., Hangzhou, China 5. NDFOS, Eumseong, Korea	Up to 40	Rapid	1141	407	734	
Shah et al. [144]	USA	N	nsp	LFIA	BinaxNOW COVID-19 Ag	Abbott	20–30	Rapid	2110	334	1776	
McKay [145]	USA	N	nsp	LFIA/virus culture data	BinaxNOW Rapid Antigen Test	Abbott	Up to 40	Rapid	532	105	427	
Yin et al. [146]	Belgium	N	nsp	LFIA	1. Panbio™ COVID-19 Ag Rapid Test Device 2. BD Veritor™ SARS-CoV-2 3. COVID-19 Ag Respi-Strip 4. SARS-CoV-2 Rapid Antigen Test	1. Abbott Rapid Diagnostics, Germany 2. Becton-Dickinson and Company, USA 3. Coris BioConcept, Belgium 4. SD Biosensor, Republic of Korea	30–40	Rapid	760	722	38	
Baro et al. [147]	Spain	N	nsp	LFIA	1. PanBioTM COVID-19 Ag Rapid test	1. Abbott 2. Siemens 3. Roche	Up to 30	Rapid	286	101	185	

					2. CLINITEST® Rapid COVID-19 Antigen Test 3. SARS-CoV-2 Rapid Antigen Test 4. SARS-CoV-2 Anti- gen Rapid Test Kit 5. COVID-19 Coro- navirus Rapid Anti- gen Test Cassette	4. Lepu Medica 5. Surescreen					
Caputo et al. [148]	Italy	N	nsp-ts	CLEIA	Lumipulse G Sars- CoV-2 Ag	Fujirebio, Tokio, Ja- pan	Up to 40	Quick/detector	4266	503	3763
Kenyeres et al. [149]	Hungary	N	nsp	LFIA	BIOCREDIT COVID- 19 Ag	RapiGEN Inc.	Up to 30	Rapid	37	37	NA
Häuser et al. [150]	Germany	N	nsp	CLEIA/virus culture data	LIAISON SARS- CoV-2 antigen test	Diasorin	20–30	Detector	196	196	27
Lefever et al. [151]	Belgium	N	nsp	LFIA/virus culture data	Liaison antigen test	Diasorin	20–30	Rapid	410	200	210
Zacharias et al. [152]	Austria	N	nsp	LFIA	SARS-CoV-2 RAT	Roche	30–40	Rapid	30	24	6
Oh et al. [153]	Korea	N	nsp	LFIA	Standard Q COVID- 19 Ag	SD Biosensor, Inc. Gyeonggi-do, Korea	Up to 30	Rapid	118	26	92
Asai et al. [154]	Japan	N	nsp	CLEIA	LUMIPULSE SARS- CoV-2 antigen kit	Fujirebio, Japan	30–40	Detector	305	63	242
Kweon et al. [155]	Korea	N	nsp	LFIA	1. AFIAS COVID-19 Ag 2. ichroma™ COVID-19 Ag	1. Boditech Med., Chuncheon-si, Gang- won-do, Republic of Korea 2. Boditech Med.	Up to 30/Up to 40/30–40	Rapid	167	167	NA
Menchinelli et al. [156]	Italy	N	nsp	CLEIA/virus culture data	LUMIPULSE SARS- CoV-2 antigen kit	Fujirebio, Japan	Up to 20/Up to 30/Up to 40/0– 20/20–30/30–40	Detector	594	194	400
Sood et al. [157]	USA	N	nsp	LFIA	BinaxNOW rapid an- tigen test	Abbott	20–30	Rapid	774	226	548
Epstude et al. [158]	Germany	N	nsp	LFIA	SARS-CoV-2 Rapid Antigen test	Roche®	Up to 40	Rapid	30	30	NA

Smith et al. [91]	USA	N	nsp	FIA/virus culture data	SARS Sofia FIA rapid antigen tests	Quidel	Up to 40	Rapid/detector	286	286	NA
Berger et al. [159]	Switzerland	N	nsp	LFIA/virus culture data	1. Panbio™ COVID-19 Ag Rapid Test device 2. Standard Q Ag-RDT	1. Abbott 2. SD Biosensor, Roche	20–30	Rapid	1064	315	749
Matsuda et al. [160]	Brazil	N	nsp	LFIA	1. COVID-19 Ag ECO Test 2. Panbio COVID-19 Ag Rapid Test	1. ECO Diagnóstica 2. Abbott, Ludwigshafen, Germany	Up to 40	Rapid	108	29	80
Van Honacker et al. [161]	Belgium	N	nsp	LFIA	1. COVID-19 ag BSS 2. SARS-CoV-2 Ag card 3. Coronavirus AG Rapid test cassette 4. Panbio COVID-19 Ag Rapid Test Device 5. SARS-CoV-2 Rapid Antigen test	1. Biosynex, Fribourg, Switzerland 2. Biotical health, Madrid, Spain 3. Zhejiang Orient Gene Biotech Co., Zhejiang, China 4. Abbott, Ludwigshafen, Germany 5. SD Biosensor, Gyeonggi-do, Korea	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	98	58	40
Boum et al. [162]	Cameroon	N	nsp	LFIA	SARS-CoV-2 Rapid Antigen test	SD Biosensor	20–30	Rapid	1090	291	799
Mboumba Bouassa et al. [163]	France	N	nsp	LFIA	SIENNA™ COVID-19 Antigen Rapid Test Cassette	Salofa Oy, Salo, Finland; manufactured under license of T&D Diagnostics Canada Pvt. Ltd., Halifax, Canada	Up to 20/Up to 40	Rapid	150	100	50
Stokes et al. [164]	Canada	N	1. nsp 2. ts	LFIA	Panbio COVID-19 antigen Rapid Test Device	Abbott, IL, USA	Up to 40	Rapid	1888	497	1391
Landaas et al. [165]	Norway	N	nsp-ts	LFIA	Panbio™ COVID-19 Ag Rapid Test Device	Abbott	Up to 30/Up to 40/30–40	Rapid	3991	250	3741

Takeuchi et al. [166]	Japan	N	nsp	LFIA/virus culture data	QuickNavi™-COVID19 Ag	Denka Co., Ltd., Tokyo, Japan	Up to 40	Rapid	1186	105	1081
Igloi et al. [167]	Netherlands	N	nsp	LFIA/virus culture data	Roche SD Biosensor SARS-CoV-2 rapid antigen test	Roche Diagnostics	Up to 30/Up to 40/30–40	Rapid	970	186	784
Masiá et al. [168]	Spain	N	1. nsp 2. ts	LFIA	Panbio COVID-19 antigen Rapid Test Device	Abbott Rapid Diagnostic Jena GmbH, Jena, Germany	Up to 40	Rapid	2174	448	1726
Jääskeläinen et al. [169]	Finland	N	nsp	1. FIA 2. LFIA/virus culture data	1. Quidel Sofia SARS FIA 2. Standard Q COVID-19 Ag test 3. Panbio™	1. Quidel, San Diego, CA 2. SD Biosensor, Republic of Korea 3. Abbott Diagnostic GmbH, Jena, Germany	Up to 30/Up to 40/30–40	1. Rapid/detector 2. Rapid 3. Rapid	198	185	40
Oleáro et al. [170]	Germany	N	nsp	LFIA/virus culture data	1. SARS-CoV-2 Rapid Antigen Test (Roche) 2. COVID-19 Rapid Test Device (Abbott) 3. MEDsan SARS-CoV-2 Antigen Rapid Test 4. CLINITEST Rapid COVID-19 Antigen Test	1. Roche Diagnostics SD Biosensor Korea 2. Abbott Rapid Diagnostics Panbio Ltd. Australia 3. MEDsan GmbH Germany 4. Zhejiang Orient Biotech Co. China	Up to 40	Rapid	184	84	100
Toshiaki Ishii et al. [171]	Japan	N	1. nsp 2. ts	1. LFIA 2. CLEIA	1. Espline® SARS-CoV-2 2. Lumipulse® SARS-CoV-2	1. Fujirebio Inc., Tokyo, Japan 2. Fujirebio Inc., Tokyo, Japan	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	1. Rapid 2. Quick/detector	893	44	849
Peña-Rodríguez et al. [172]	Mexico	N	nsp	LFIA	STANDARD™ Q COVID-19 Ag Test	SD BIOSENSOR	Up to 40	Rapid	369	104	265
Gili et al. [173]	Italy	N	nsp	CLEIA	Lumipulse® SARS-CoV-2 antigen assay	Fujirebio, Inc., Tokyo, Japan	Up to 40	Quick/detector	1964	185	1779

Pérez-García et al. [174]	Spain	N	nsp	LFIA	1. CerTest SARS-CoV-2 Ag One Step Card Test 2. Panbio COVID-19 Ag Rapid Test Device	1. Certest Biotec S. L., Zaragoza, Spain) 2. Abbot Rapid Diagnostics GmbH, Jena, Germany	Up to 30/Up to 40/30–40	Rapid	320	170	150
Kilic et al. [175]	USA	N	nsp	LFIA	BD Veritor SARS-CoV-2	Becton, Dickinson, Sparks, MD, USA	Up to 40	Rapid	1384	116	1268
Drain et al. [176]	USA	N	nsp	FIA	LumiraDx SARS-CoV-2 antigen test	LumiraDx UK Ltd., Dumyat Business Park, Alloa, FK10 2PB, UK)	Up to 40	Rapid/detector	512	123	389
Basso et al. [177]	Italy	N	1. nsp 2. ts	1. LFIA 2. LFIA 3. CLEIA	1. ESPLINE rapid test 2. COVID-19 Ag Rapid Test 3. Lumipulse G Sars-CoV-2 Ag	1. Fujirebio 2. ABBOTT 3. Fujirebio	Up to 40	1. Rapid 2. Rapid 3. Quick/detector	234	87	147
Pollock et al. [178]	USA	N	nsp	LFIA	BinaxNOW COVID-19 Ag card	Abbott Diagnostics Scarborough, Inc.	Up to 30/Up to 40/30–40	Rapid	2307	292	2015
Ristić et al. [179]	Serbia	N	nsp	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Gyeonggi-do, Korea	Up to 40	Rapid	120	43	77
Courtellemont et al. [180]	France	N	nsp	LFIA	COVID-VIRO®	AAZ, Boulogne Billancourt, France	Up to 30/Up to 40/30–40	Rapid	248	121	127
Thommes et al. [181]	Austria	N	nsp	LFIA	1. Panbio™ COVID-19 Ag Rapid test 2. Novel Coronavirus (2019-nCov) Antigen Detection Kit 3. DIAQUICK COVID-19 Ag Cassette 4. SARS-CoV-2 Rapid Antigen Test	1. Abbott, Chicago, Illinois 2. CLMSRDL, Sichuan Mass Spectrometry Biotechnology Co., Ltd., Chengdu, Sichuan 3. DIALAB, Wiener Neudorf, Austria 4. Roche Diagnostics Deutschland GmbH,	Up to 30/Up to 40/30–40	Rapid	154	154	NA

					Mannheim, Germany						
González-Donapetry et al. [182]	Spain	N	nsp	LFIA	Panbio COVID-19 Ag Rapid Test Device	Abbott Rapid Diagnostics Jena GmbH, Jena, Germany	Up to 40	Rapid	440	18	422
Eshghifar et al. [183]	?	N	ts	LFIA	1. BD Veritor™ System for rapid detection of SARS-CoV-2 2. CareStart™ COVID-19 Antigen 3. SG Diagnostics Antigen detection kit 4. Sofia SARS Antigen FIA 5. Rapid Response™ COVID-19 Antigen Rapid Test 6. Shenzhen SARS-CoV-2 Antigen Test kit 7. Genedia W COVID-19 Ag	1. Becton, Dickinson and Company, MD, USA 2. Accesas Bio, Inc., NJ, USA 3. SG Diagnostics, Singapore 4. Quedel Corporation, Hannover, Germany 5. BNTX, Inc., ON, Canada 6. Shenzhen Ultra-Diagnostics Biotech. Co., Ltd., Shenzhen, PRC 7. Green Cross Medical Sciences Corp., Chungcheongbuk, Republic of Korea	Up to 40	Rapid	5	5	NA
Merino et al. [184]	Spain	N	nsp	LFIA	Panbio™ COVID-19 Ag Rapid Test Device	Abbott Diagnostic GmbH, Jena, Germany	Up to 30/Up to 40/30–40	Rapid	958	359	599
Shao et al. [38]	USA	1. N 2. S	nsp	FET	In-house		Up to 40	NA/detector	38	28	10
Bulilete et al. [185]	Spain	N	nsp	LFIA	Panbio™ Ag-RDT	Abbott Diagnostic GmbH, Jena, Germany	Up to 40	Rapid	1367	140	1222
Torres et al. [186]	Spain	N	nsp	LFIA/virus culture data	CLINITEST® Rapid COVID-19 Antigen Test	Siemens, Healthineers, Erlangen, Germany	Up to 40	Rapid	270	116	154

Lindner et al. [187]	Germany	N	nsp	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	179	41	138
Hirotsu et al. [188]	Japan	N	nsp	CLEIA	LUMIPULSE SARS-CoV-2 antigen test	Fujirebio, Inc., Tokyo, Japan)	Up to 40	Detector	1029	40	989
Salvagno et al. [189]	Italy	N	nsp-ts	LFIA	Roche SARS-CoV-2 Rapid Antigen Test	Roche Diagnostics, Basel, Switzerland	Up to 40	Rapid	321	149	172
Veyrenche et al. [190]	France	N	nsp	LFIA	Coris COVID-19 Ag Respi-Strip	BioConcept	Up to 30/Up to 40/30–40	Rapid	65	45	20
Porte et al. [191]	Chile	N	nsp	FIA	1. SOFIA SARS Antigen FIA 2. STANDARD F COVID-19 Ag FIA	1. Quidel Corporation, San Diego, CA, USA 2. SD Biosensor Inc., Gyeonggi-do, Republic of Korea	Up to 40	Rapid/detector	64	32	32
Domínguez Fernández et al. [192]	Spain	N	nsp	LFIA	Panbio™ rapid antigens test device	Abbott	Up to 40	Rapid	30	20	10
Kobayashi et al. [193]	Japan	N	nsp	1. CLEIA 2. LFIA	1. Lumipulse Presto SARS-CoV-2 Ag 2. Espline SARS-CoV-2	1. Fujirebio Inc., Tokyo, Japan 2. Fujirebio Inc., Tokyo, Japan	Up to 40	1. Quick/detector 2. Rapid	300	100	200
Houston et al. [194]	UK	N	nsp	LFIA	Innova SARS-CoV-2 Antigen Rapid Qualitative Test	Lotus Global Company, London, UK	Up to 40	Rapid	728	280	448
Gremmels et al. [73]	Netherlands/Aruba	N	nsp	LFIA	Panbio™ COVID-19 antigen	Abbott (Lake County, IL, USA)	Up to 40	Rapid	1573	202	1371
Ciotti et al. [195]	Italy	N	nsp	LFIA	Coris COVID-19 Ag Respi-Strip	Coris BioConcept	Up to 40	Rapid	50	39	11
Okoye et al. [196]	USA	N	nsp	LFIA	Abbott BinaxNOW COVID-19 antigen card	Abbott Diagnostics Scarborough, Inc.	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	2638	45	2593
Kurtulmus et al. [47]	Turkey	N	urine	UFT	In-house		Up to 40	Rapid	201	86	115

Saadi et al. [37]	France	N	nsp	1. LFIA 2. LFIA 3. LC-MS	1. NG Test Ag 2. COVID-19 Ag Respi-Strip 3. In-house	1. NG Biotech, France 2. Coris, Belgium	Up to 20/Up to 30/Up to 40/0– 20/20–30/30–40	1. Rapid 2. Rapid 3. NA/detector	19	12	7
James et al. [197]	USA	N	nsp	LFIA	BinaxNOW COVID- 19 Ag Card tests	Abbott Diagnostics, Scarborough	Up to 40	Rapid	2339	152	2187
Villaverde et al. [198]	Spain	N	nsp	LFIA	Panbio COVID-19 Ag Rapid Test	Abbott Rapid Diag- nostic	Up to 40	Rapid	1620	77	1543
Pekosz et al. [199]	USA	N	nsp	LFIA/virus culture data	BD Veritor Antigen Test	Becton, Dickinson and Company, BD Life Sciences–, San Diego, California	Up to 40	Rapid	38	38	NA
Kohmer et al. [200]	Germany	N	nsp	LFIA/virus culture data	1. RIDA®QUICK SARS-CoV-2 Anti- gen 2. SARS-CoV-2 Rapid Antigen Test 3. NADAL® COVID- 19 Ag Test (test cas- sette) 4. LumiraDx™ Plat- form SARS-CoV-2 Ag Test	1. R-Biopharm AG, Darmstadt, Germany 2. Roche Diagnostics GmbH, Mannheim, Germany 3. Nal von Minden GmbH, Regensburg, Germany) 4. LumiraDx GmbH, Cologne, Germany	Up to 40	Rapid	100	74	26
Prince-Guerra et al. [201]	USA	N	nsp	LFIA/virus culture data	BinaxNOW COVID- 19 Ag Card	Abbott Diagnostics Scarborough, Inc.	Up to 40	Rapid	3419	299	3120
Möckel et al. [202]	Germany	N	nsp	LFIA/virus culture data	Roche SARS-CoV-2 rapid antigen test	SD Biosensor	Up to 40	Rapid	271	89	182
Rottenstreich et al. [203]	Israel	N	nsp	LFIA	NowCheck COVID- 19 Ag Test	Bionote Inc., Hwaseong-si, Re- public of Korea	Up to 30/Up to 40/30–40	Rapid	1326	9	1317
Favresse et al. [204]	Belgium	N	nsp	1. LFIA 2. LFIA 3. LFIA 4. LFIA 5. CLEIA	1. Biotical SARS- CoV-2 Ag card 2. Panbio™ COVID- 19 Ag Rapid Test De- vice	1. Biotical Health, Madrid, Spain 2. Abbott, Chicago, IL, USA 3. Healgen Scientific, Houston, TX, USA	Up to 20/Up to 30/Up to 40/0– 20/20–30/30–40	1. Rapid 2. Rapid 3. Rapid 4. Rapid 5. Quick/detector	188	96	92

					3. Coronavirus Ag Rapid Test Cassette 4. Roche SARS-CoV-2 Rapid Antigen Test 5. VITROS Immuno-diagnostic Products SARS-CoV-2 Antigen test	4. Roche Diagnostics, Basel, Switzerland 5. Ortho Clinical Diagnostics, Raritan, NJ, USA					
Osterman et al. [205]	Germany	N	nsp-ts	1. LFIA 2. FIA	1. SARS-CoV-2 Rapid Antigen Test 2. STANDARD™ F COVID-19 Ag	1. SD Biosensor, Suwon, Korea 2. Roche, Switzerland	Up to 40	1. Rapid 2. Rapid/detector	1572	826	746
Pollock et al. [206]	USA	N	nsp	CLEIA/virus culture data	MSD S-PLEX SARS-CoV-2 N assay	MSD Meso Scale Discovery [MSD]	Up to 40	Quick/detector	226	136	90
Aoki et al. [207]	Japan	N	nsp	CLEIA	Lumipulse® SARS-CoV-2 Ag	Fujirebio Inc., Tokyo, Japan	Up to 40	Quick/detector	548	30	518
Torres et al. [208]	Spain	N	nsp	LFIA	Panbio™ COVID-19 Ag	Abbott Diagnostics, Jena, Germany	Up to 40	Rapid	634	79	555
Aleman et al. [209]	Spain	N	nsp	LFIA	Panbio COVID-19 Ag Test	Abbott Rapid Diagnostics, Germany	Up to 30/Up to 40/30–40	Rapid	1406	951	455
Rastawicki et al. [210]	Poland	N	nsp	FIA	PCL COVID-19 Ag	PCL Inc., Korea	Up to 40	Rapid	42	36	6
Yamamoto et al. [211]	Japan	N	nsp	LFIA	ESPLINE SARS-CoV-2	Fujirebio Inc., Japan	Up to 40	Rapid	229	128	101
Kashiwagi et al. [212]	Japan	N	1. ts 2. nsp	LFIA	ESPLINE® SARS-CoV-2	Fujirebio Inc., Tokyo	Up to 40	Rapid	6	4	2
Pilarowski et al. [213]	USA	N	nsp	LFIA/virus culture data	BinaxNOW rapid antigen test	Abbott Diagnostics Scarborough, Inc.	Up to 30/Up to 40/30–40	Rapid	871	26	845
Aoki et al. [214]	Japan	N	nsp	LFIA	Espline® SARS-CoV-2	Fujirebio Inc., Japan	Up to 40	Rapid	129	63	66
Pray et al. [215]	Wisconsin	N	nsp	FIA/virus culture data	Sofia SARS Antigen	Quidel Corporation	Up to 40	Rapid/detector	1098	57	1041
Strömer et al. [216]	Germany	N	nsp	LFIA/virus culture data	1. NADAL® COVID-19 Ag Test 2. Panbio™ COVID-19 Antigen	Nal von Minden GmbH, Moers, Germany Abbott Rapid Diagnostics, Germany	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	124	124	NA

Toptan et al. [217]	Germany	N	nsp-ts	LFIA/virus culture data	novel antigen test	R-Biopharm	Up to 40	Rapid	67	58	9
Turcato et al. [218]	Italy	N	ts	LFIA	STANDARD Q COVID-19 Ag (R-Ag)	SD BIOSENSOR, KR	Up to 40	Rapid	3410	223	3187
Mak et al. [219]	Hong Kong	N	1. nsp-ts 2. nsp 3. ts	LFIA/virus culture data	Panbio COVID-19 Ag Rapid Test Device	Abbott Rapid Diagnostics, Germany	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	35	8	27
Zhang et al. [220]	China	N	nsp-ts	FIA/virus culture data	SARS-CoV-2 N-protein test strip	Beijing Savant Biotechnology Co., Ltd.	Up to 40	Rapid/detector	547	247	300
Agulló et al. [221]	Spain	N	1. nsp 2. ts 3. nsp-ts	LFIA	Panbio COVID-19 Ag-RDT	Abbott Rapid Diagnostic Jena GmbH, Jena, Germany)	Up to 40	Rapid	659	126	527
Tanimoto et al. [222]	Japan	N	nsp	LFIA	ESPLINE SARS-CoV-2®	Fujirebio Inc., Tokyo, Japan	Up to 40	Rapid	8	2	6
Lindner et al. [223]	Germany	N	nsp	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 20/Up to 30/Up to 40/0–20/20–30/30–40	Rapid	39	39	NA
Abdelrazik et al. [224]	Egypt	N	nsp	LFIA	BIOCREDIT COVID-19 Ag test	RapiGEN Inc.	Up to 30/Up to 40/30–40	Rapid	188	188	NA
Weitzel et al. [225]	Chile	N	1. nsp-ts 2. nsp	1. LFIA 2. FIA 3. FIA	1. Biocredit One Step SARS-CoV-2 Antigen Test 2. Huaketai New Coronavirus (SARS-CoV-2) N Protein Detection Kit (FIA) 3. Diagnostic Kit for 2019-Novel Coronavirus (2019-nCoV)	1. RapiGen Inc., Anyang-si, Gyeonggi-do, Rep. of Korea 2. Savant Biotechnology Co., Beijing, China 3. Bioeasy Biotechnology Co., Shenzhen, China	Up to 40	1. Rapid 2. Rapid/detector 3. Rapid/detector	111	80	31
Winkel et al. [226]	Netherlands	N	nsp	LFIA	PanbioTM COVID-19 Ag	Abbott	Up to 40	Rapid	2390	63	2327
Hoehl et al. [227]	Germany	N	nsp	LFIA	RIDA® QUICK SARS80 CoV-2 Antigen test	R-Biopharm	Up to 20	Rapid	602	8	594

Priya Kannian et al. [228]	India	N	nsp	LFIA	SARS-CoV2 antigen kit	SD Biosensor	Up to 40	Rapid	30	20	10
Lindner et al. [229]	Germany	N	nsp	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc., Gyeonggi-do, Korea	Up to 40	Rapid	146	40	106
Filgueiras et al. [230]	Brazil	N	nsp	LFIA	SARS-CoV-2 rapid antigen test	ECODiagnostica	Up to 40	Rapid	139	55	84
Peto et al. [231]	UK	N	nsp-ts	LFIA	SARS-CoV-2 Antigen Rapid Qualitative Test	Innova	Up to 30	Rapid	834	198	636
Jakobsen et al. [232]	Denmark	N	nsp	LFIA	STANDARD Q COVID-19 Ag test	SD BIOSENSOR	Up to 40	Rapid	4811	221	4590
Miyakawa et al. [233]	Japan	N	nsp	LFIA/virus culture data	1. SARS-CoV-2 Ag-RDT		Up to 40	Rapid	108	45	63
					2. Panbio COVID-19 Ag Rapid Test	1. YCU-FF					
					3. SARS-CoV-2 Rapid Antigen Test	2. Abbott					
					4. SD Biosensor Standard Q COVID-19 Ag	3. Roche					
					5. Espline SARS-CoV-2	4. SD Bio					
						5. Fujirebio					
Torres et al. [186]	Spain	N	nsp	LFIA/virus culture data	CLINITEST® Rapid 29 COVID-19 Antigen Test	Siemens, Healthineers, Erlangen, Germany	Up to 40	Rapid	270	33	237
Pollock et al. [234]	Massachusetts	N	nsp	LFIA	Access Bio CareStart COVID-19 Antigen test		Up to 30/Up to 40	Rapid	1498	234	1264
Shidlovskaya et al. [235]	Russia	N	nsp	LFIA/virus culture data	1. SGTI-flex COVID-19 Ag 2. Biocredit COVID-19 Ag	1. SUGENTECH, INC 3. RapiGEN Inc.	Up to 40	Rapid	106	14	92
Faíco-Filho et al. [236]	Brazil	N	nsp	LFIA	Panbio™ COVID-19 Ag Rapid Test	Abbott	Up to 30/Up to 40/30–40	Rapid	127	70	57

Schuit et al. [237]	Netherlands	N	nsp	LFIA/virus culture data	1. BD Veritor™ System Ag-RDT 2. SD Biosensor Ag-RDT	1. Becton, Dickinson and Company, Franklin Lakes, NJ, USA 2. Roche	Up to 40	Rapid	4274	365	4274
Ducrest et al. [238]	Switzerland	N	nsp	LFIA	COVIDia-Antigen	GaDia SA	Up to 30	Rapid	60	20	40
Vecchio et al. [239]	Italy	N	nsp	LFIA	Panbio™ COVID-19 Ag test	Abbott	Up to 30	Rapid	1441	61	1380
Bonde et al. [240]	Denmark	N	ts	LFIA	BD VERITOR Ag Rapid test	Becton-Dickinson and Company, USA	Up to 30	Rapid	809	65	744
Igloi et al. [241]	Netherlands	N	ts	LFIA/virus culture data	SARS-CoV-2 Rapid Antigen Test	Distributed by Roche (SD Biosensor)	Up to 30	Rapid	770	30	740
Thell et al. [242]	Austria	N	nsp	LFIA	SARS-CoV-2 Rapid Antigen Test	Roche Diagnostics	Up to 30	Rapid	541	213	328
Pollock et al. [243]	Massachusetts	N	nsp	LFIA	BinaxNOW COVID-19 Ag	Abbott	Up to 30	Rapid	98	98	NA
Hagbom et al. [244]	Sweden	N	ts	LFIA/virus culture data	1. Rapid Response™ COVID-19 Antigen Rapid Test Cassette for oral fluids 2. DIAGNOS™ COVID-19 Antigen Saliva Test	1. BioServ 2. DIAGNOS	Up to 30	Rapid	34	15	19
Thirion-Romero et al. [245]	Mexico	N	nsp	LFIA	Panbio™	Abbott	Up to 30	Rapid	1064	474	590
Chiu et al. [246]	Hong Kong	N	nsp	LFIA	INDICAID™ Rapid Test	PHASE Scientific i	Up to 30	Rapid	23,343	128	23,215
Abusrewil et al. [247]	Libya	N	nsp	LFIA	1. SARS-CoV-2 spike protein test 2. Shenzhen Micro-profit Biotech Co 3. ESPLINE SARS-CoV-2	1. Fluorecare 2. Biotech 3. Fujirebio 4. Biocredit 5. Abbott 6. Acon 7. Assut	Up to 30/Up to 40	Rapid	231	83	145

					4. RapiGen COVID-19 Ag Detection Kit 5. Panbio™ COVID-19 Ag Rapid Test 6. Flowflex™ SARS-CoV-2 Antigen Rapid Test 7. Europe antigen testing COVID-19 8. Bioperfectus SARSCoV-2 Antigen Rapid Test Kit 9. AMP Rapid Test SARS-CoV-2 Ag 10. Coronavirus ag rapid test cassette	8. BIOPERFECTUS 9. AMP 10. Orient GENE					
Muthamia et al. [248]	Kenya	N	nsp	LFIA	BD Veritor antigen test	Becton-Dickinson and Company, USA	Up to 20/Up to 30/0–20/20–30	Rapid	272	47	225
Abdul-Mumin et al. [249]	Ghana	N	nsp	LFIA	STANDARD Q SARS-CoV-2 Ag Test	SD Biosensor	Up to 40	Rapid	193	42	151
Akashi et al. [250]	Japan	N	nsp	LFIA	QuickNavi™-COVID19 Ag	Otsuka Pharmaceutical Co., Ltd. (Otsuka) and Denka Company	Up to 40	Rapid	96	96	NA
Lindner et al. [251]	Germany	N	nsp	LFIA	1. Espline SARS-CoV-2 2. Sure Status COVID-19 Antigen Card Test 3. Mologic COVID-19 Rapid Test	1. Fujirebio Inc. 2. Premier Medical Corporation Private Limited 3. Fujirebio Inc	Up to 40	Rapid	329	329	NA
Suliman et al. [252]	Massachusetts	N	nsp	LFIA	Access Bio CareStart™ COVID-19 RDT	CareStart	Up to 30	Rapid	631	37	594

Bruins et al. [253]	Nether-lands	N	nsp	LFIA	Panbio™ COVID-19 Ag Rapid Test	Abbott	Up to 30	Rapid	1101	84	917
Ford et al. [254]	Wisconsin	N	nsp	LFIA/virus culture data	BinaxNOW SARS-CoV-2 antigen test	Abbott Laboratories, Abbott Park, IL	Up to 40	Rapid	2110	334	1776
Koskinen et al. [255]	Finland	N	nsp	LFIA/virus culture data	mariPOC SARS-CoV-2 Antigen Test	mariPOC	Up to 30	Rapid/optional de-tector	211	13	198
Nikolai et al. [256]	Germany	N	nsp	LFIA	STANDARD Q COVID-19 Ag Test	SD Biosensor, Inc. Gyeonggi-do, Korea	Up to 40	Rapid	228	70	188
Stohr et al. [257]	Nether-lands	N	nsp	LFIA/virus culture data	1. BD Veritor System for Rapid Detection of SARS-CoV-2 2. Roche SARS-CoV-2 antigen detection test	Becton Dickinson company, USA Roche, Switzerland	Up to 40	Rapid	3239	454	1528

LFIA: Lateral Flow Immunoassay; FIA: Fluorescence Immunoassay; CLEIA: Chemiluminescence Enzyme Immunoassay; FET: Field-Effect Transistors; Ag: Anti-gen; nsp: nasopharyngeal; ts: oropharyngeal/throat/saliva; Rapid: detection time 5-20 minutes (mainly 15) but never exceeding 30 minutes; Quick: detection time 30-35 minutes; Quick *: 60 minutes; w/wo: with/without; Detector: a detector is needed to read the developed signal; NA: Not applicable; NR: Not reported; Cases: SARS-CoV-2 positive samples according to RT-PCR; Controls: healthy individuals and RT-PCR negative (for SARS-CoV-2); Virus culture data: study that provides any kind of data on the correlation between virus culture [cytopathic effect, tissue culture infective dose 50% (TCID₅₀), limit of detection (LoD)], and rapid Antigen Test positivity, RNA copies number, Ct values of RT-PCR positive samples.

3.2. Analysis of Diagnostic Performance

A great amount of the available data, for all methods, concerned samples detected with qPCR Ct values of 20, and mostly of 30 and 40. As shown in Table 2, the sensitivity of LFIA tests (using the N antigen) based on NSP samples that were qPCR-positive for Ct < 20 was 0.945 (95% CI: 0.930, 0.961). It declined, however, considerably to 0.329 (95% CI: 0.265, 0.393) for 30 < Ct < 40. LFIA tests using TS samples performed worse in terms of sensitivity, with a highest estimate of 0.805 (95% CI: 0.599, 1.000) in samples positive for Ct < 20 and a lowest of 0.085 (0.000, 0.176) for Ct > 30 (Table 2). The specificity of LFIA on NSP and TS samples (using the N antigen) was very high across all Ct intervals, ranging from 0.959 (95% CI: 0.923, 0.995) to 0.996 (95% CI: 0.993, 0.998). The sensitivity of FIA (using the N antigen) on NSP samples also showed a declining pattern from 0.935 (95% CI: 0.880, 0.990) for Ct < 20 to 0.435 (95% CI: 0.190, 0.680) for 30 < Ct < 40. Specificity was also very high using NSP qPCR positive samples for Ct < 30 (0.992, 95%: 0.979, 1.000). CLEIA (using the N antigen) had high sensitivity based on NSP samples that were PCR-positive for Ct < 30 (0.980, 95% CI: 0.960, 0.999); this estimate, however, was based on a smaller number of studies and dropped considerably at higher Ct (30–40) values (0.515; 95% CI: 0.220, 0.810). The specificity of CLEIA was very high in all comparisons. The evaluation of the performance of other methods (using the N antigen) on NSP and TS samples for the above studied Ct values intervals (0–20, 21–30, and 31–40) was based on a few studies but showed similar patterns. Data on methods using other antigens (i.e., based on S, E or M protein) were too scarce to allow reliable estimations (Table 2).

Table 2. Results of the multivariate meta-analysis for the different types of assays using different samples and stratified according to different cut-off rt-PCR values. Listed information includes the pooled sensitivity and specificity along with the 95% confidence intervals (NSP: pharyngeal, nasopharyngeal, nasal specimens, TS: throat, saliva, N: nucleocapsid protein, S: spike protein, M: membrane E: envelope, NS: nucleocapsid and Spike proteins).

Sample	Ag	Method	Ct Values	Studies/Patients/ Controls	Sensitivity (95% CI)	Specificity (95% CI)	Studies w/o Con- trols
NSP	N	LFIA	0–20	41/7464/3945	0.945 (0.930, 0.961)	0.993 (0.987, 0.998)	22
NSP	N	LFIA	0–30	99/66,939/47,719	0.853 (0.826, 0.879)	0.991 (0.988, 0.995)	44
NSP	N	LFIA	0–40	207/88,008/69,415	0.702 (0.676, 0.727)	0.990 (0.987, 0.993)	30
NSP	N	LFIA	20–30	46/7817/4360	0.790 (0.739, 0.841)	0.987 (0.976, 0.998)	35
NSP	N	LFIA	30–40	71/5150/911	0.329 (0.265, 0.393)	0.959 (0.923, 0.995)	51
TS	N	LFIA	0–20	5/90/NA	0.805 (0.599, 1.000)	-	5
TS	N	LFIA	0–30	10/2136/1756	0.636 (0.477, 0.795)	0.994 (0.989, 0.998)	5
TS	N	LFIA	0–40	23/10,249/9232	0.354 (0.238, 0.470)	0.996 (0.993, 0.998)	12
TS	N	LFIA	20–30	6/160/NA	0.394 (0.086, 0.702)	-	6
TS	N	LFIA	30–40	4/44/NA	0.085 (0.000, 0.176)	-	4
NSP-TS	N	LFIA	0–20	7/4240/3859	0.999 (0.000, 1.000)	0.999 (0.000, 1.000)	6
NSP-TS	N	LFIA	0–30	12/9229/8133	0.867 (0.792, 0.942)	0.999 (0.997, 1.000)	10
NSP-TS	N	LFIA	0–40	30/23,970/21,699	0.696 (0.638, 0.754)	0.992 (0.987, 0.996)	4
NSP-TS	N	LFIA	20–30	10/1995/1504	0.575 (0.279, 0.870)	0.997 (0.987, 1.000)	7
NSP-TS	N	LFIA	30–40	10/217/NA	0.417 (0.242, 0.593)	-	9
NSP	N	FIA	0–20	3/97/NA	0.935 (0.880, 0.990)	-	3
NSP	N	FIA	0–30	10/2221/421	0.807 (0.726, 0.889)	0.992 (0.979, 1.000)	6
NSP	N	FIA	0–40	29/36,425/33,718	0.707 (0.631, 0.783)	0.984 (0.970, 0.997)	1
NSP	N	FIA	20–30	3/598/NA	0.729 (0.544, 0.915)	-	3
NSP	N	FIA	30–40	12/2283/665	0.435 (0.190, 0.680)	0.983 (0.971, 0.995)	9
TS	N	FIA	0–40	2/114/31	0.162 (0.083, 0.241)	0.984 (0.941, 1.000)	1
NSP-TS	N	FIA	0–30	4/195/77	0.944 (0.904, 0.985)	0.975 (0.944, 1.000)	1
NSP-TS	N	FIA	0–40	11/2779/2018	0.691 (0.520, 0.862)	0.971 (0.953, 0.989)	2
NSP-TS	N	FIA	30–40	3/72/32	0.792 (0.434, 1.000)	0.969 (0.926, 1.000)	1
NSP	N	CLEIA	0–20	3/789/152	0.955 (0.907, 1.000)	0.997 (0.000, 1.000)	2

NSP	N	CLEIA	0–30	3/1268/111	0.980 (0.960, 0.999)	0.995 (0.000, 1.000)	2
NSP	N	CLEIA	0–40	21/7626/5910	0.818 (0.774, 0.862)	0.978 (0.968, 0.988)	1
NSP	N	CLEIA	20–30	4/378/68	0.900 (0.672, 1.000)	0.986 (0.960, 1.000)	2
NSP	N	CLEIA	30–40	4/416/261	0.515 (0.220, 0.810)	0.978 (0.957, 0.999)	2
TS	N	CLEIA	0–20	1/136/NA	0.875 (0.550, 1.000)	-	1
TS	N	CLEIA	0–30	1/136/NA	0.928 (0.738, 1.000)	-	1
TS	N	CLEIA	0–40	3/376/179	0.709 (0.359, 1.000)	0.977 (0.950, 1.000)	1
TS	N	CLEIA	20–30	1/3/NA	0.875 (0.550, 1.000)	-	1
TS	N	CLEIA	30–40	1/3/NA	0.667 (0.000, 1.000)	-	1
NSP-TS	N	CLEIA	0–40	1/4266/3763	0.867 (0.837, 0.896)	0.973 (0.968, 0.978)	0
NSP-TS	N	CLEIA	20–30	1/978/817	0.795 (0.733, 0.857)	0.997 (0.000, 1.000)	0
NSP	N	other	0–20	2/45/7	0.973 (0.921, 1.000)	0.9375 (0.769, 1.000)	1
NSP	N	other	0–30	4/219/51	0.923 (0.807, 1.000)	0.963 (0.890, 1.000)	1
NSP	N	other	0–40	8/1228/388	0.768 (0.643, 0.894)	0.915 (0.821, 1.000)	0
NSP	N	other	20–30	2/110/NA	0.842 (0.422, 1.000)	-	2
NSP	N	other	30–40	4/73/NA	0.540 (0.147, 0.934)	-	4
NSP	S	LFIA	0–20	1/90/49	0.976 (0.928, 1.000)	0.857 (0.000, 1.000)	0
NSP	S	LFIA	0–30	2/407/234	0.783 (0.627, 0.938)	0.942 (0.833, 1.000)	0
NSP	S	LFIA	0–40	2/129/54	0.848 (0.768, 0.930)	0.862 (0.771, 0.954)	0
NSP	S	LFIA	20–30	1/80/49	0.677 (0.513, 0.842)	0.857 (0.000, 1.000)	0
NSP	S	other	0–40	4/286/207	0.872 (0.780, 0.963)	0.911 (0.761, 1.000)	0
TS	S	other	0–40	3/96/42	0.817 (0.635, 1.000)	0.931 (0.856, 1.000)	0
TS	N, S	other	0–40	1/433/397	0.986 (0.949, 1.000)	0.962 (0.943, 0.981)	0
NSP-TS	S + E + M	other	0–40	1/94/49	0.955 (0.895, 1.000)	0.959 (0.904, 1.000)	0
URINE	N, S	other, FIA	0–40	3/271/145	0.715 (0.310, 1.000)	0.869 (0.647, 1.000)	0

Combining all major methods (LFIA, FIA and CLEIA) on NSP and TS samples, measuring both N and S antigens and stratified according to two Ct values (<30 and <40), the maximum sensitivity was estimated at 0.858 (95% CI 0.835, 0.881) for NSP samples positive for Ct < 30 (Table 3). The sensitivity using qPCR positive NSP samples for Ct < 40 is lower at 0.726 (95% CI 0.706, 0.746). Again, antigen testing of NSP samples outperformed that of TS samples for both Ct < 30 and Ct < 40 (0.637 (95% CI: 0.478, 0.795) and 0.438 (95% CI: 0.332, 0.547), respectively). Specificity was very high in all meta-analyses (Table 3).

Table 3. Results of the multivariate meta-analysis performed cumulatively for methods and/or antigen tested, in <30 and <40 Ct values. Listed information includes the pooled sensitivity and specificity along with the 95% confidence intervals (NSP: pharyngeal, nasopharyngeal, nasal specimens, TS: throat, saliva, oropharyngeal, N: nucleocapsid protein, S: spike protein, M: membrane E: envelope, NS: nucleocapsid and Spike proteins).

Sample	Ag	Method (LFIA, FIA, CLEIA)	Ct Values	Studies	Sensitivity (95% CI)	Specificity (95% CI)	Studies w/o Controls
NSP	NS	LFIA or FIA or CLEIA	30	118	0.858 (0.835, 0.881)	0.991 (0.987, 0.995)	53
NSP	NS	LFIA or FIA or CLEIA	40	325	0.726 (0.706, 0.746)	0.989 (0.987, 0.992)	39
TS	NS	LFIA or FIA or CLEIA	30	10	0.637 (0.478, 0.795)	0.994 (0.989, 0.998)	5
TS	NS	LFIA or FIA or CLEIA	40	36	0.438 (0.332, 0.547)	0.993 (0.987, 0.999)	14
NSP	NS	LFIA or FIA	30	114	0.854 (0.830, 0.878)	0.991 (0.987, 0.995)	50
NSP	NS	LFIA or FIA	40	303	0.718 (0.697, 0.739)	0.989 (0.987, 0.992)	38
TS	NS	LFIA or FIA	30	10	0.637 (0.478, 0.795)	0.994 (0.989, 0.998)	5

TS	NS	LFIA or FIA	40	32	0.395 (0.285, 0.505)	0.995 (0.993, 0.997)	13
NSP	NS	LFIA	30	101	0.852 (0.825, 0.878)	0.991 (0.987, 0.995)	44
NSP	NS	LFIA	40	269	0.715 (0.692, 0.738)	0.990 (0.987, 0.992)	35
TS	NS	LFIA	30	10	0.637 (0.478, 0.795)	0.994 (0.989, 0.998)	5
TS	NS	LFIA	40	29	0.408 (0.292, 0.523)	0.995 (0.993, 0.997)	12
NSP	NS	FIA	30	13	0.868 (0.813, 0.924)	0.991 (0.981, 1.000)	6
NSP	NS	FIA	40	35	0.730 (0.674, 0.785)	0.986 (0.976, 0.995)	3
TS	NS	FIA	30	-	-	-	-
TS	NS	FIA	40	2	0.162 (0.083, 0.242)	0.984 (0.941, 1.000)	1
NSP	NS	CLEIA	30	4	0.977 (0.955, 0.998)	0.995 (0.000, 1.000)	3
NSP	NS	CLEIA	40	23	0.816 (0.761, 0.870)	0.979 (0.971, 0.988)	1
TS	NS	CLEIA	30	-	-	-	-
TS	NS	CLEIA	40	3	0.720 (0.380, 1.000)	0.957 (0.889, 1.000)	1

To attain a better insight into how each method performs, we compared the meta-analysis results for the sensitivity and specificity of each method (LFIA, FIA, CLEIA) on NSP and TS samples for all antigens cumulatively (N plus S). As shown in Table 3, in terms of sensitivity, the laboratory CLEIA method outperforms the point of care (POC) methods (LFIA and FIA), the NSP samples outperform the TS samples, and the best results are obtained for samples identified positive with PCR for Ct < 30 (0.977 (95% CI: 0.955, 0.998) versus 0.408 (95% CI: 0.292, 0.523) and 0.162 (95% CI: 0.083, 0.242)) (Table 3).

Since the ultimate goal of a diagnostic method for SARS-CoV-2 is to identify an infected person regardless of the low viral load, we compared the overall sensitivity of rapid tests performed in points either of care or where virus surveillance is performed (LFIA or FIA) with laboratory methods (CLEIA) that show the highest sensitivity. As shown in Figure 2 (and Table 3), the overall (for Ct < 40) sensitivity of POC methods is about 10% lower than that of the CLEIA method for NSP samples (0.718 (95% CI: 0.697, 0.739) compared to 0.816 (95% CI: 0.761, 0.870)). Specificity was again high in all cases ranging from 0.957 (95% CI: 0.889, 1.000) to 0.995 (95% CI: 0.993, 0.997), although due to the small number of the included studies in some subgroups, these results may have some uncertainty (Table 3).

To investigate the validity of our stratification analysis according to Ct values (<30 and <40), we tried to explore the association between a patient/sample's infectivity and positivity in POC antigen tests (LFIA and FIA) and PCR tests using data from the included studies. We found 51 studies (Table 1) that used a virus culture to address this issue; however, the results were presented in a plethora of different ways and could not be quantitatively synthesized and analyzed, due to different reported parameters. From them, ten studies used virus cultures to only test the viral load (RNA copies/mL) that a POC test could detect. The remaining 34 studies presented a combination of data such as the limit of detection (LoD) in terms of RNA copies/mL or per swab or in pfus/mL, tissue culture infection dose (TCID), TCID₅₀, TCID_{95%}, sensitivity of POC tests in correlation with virus culture cytopathic effect (CPE) measured in different days and after zero, one or two passages.

Nevertheless, sixteen studies [63,85,87,91,101,135,145,151,167,169,199,215,216,217,219,255] determined LoD Ct values ranging from 18.57 [219] to 34 [145], with most of them reporting Ct 30 as an average threshold for a POC test to be positive. Importantly, viral culture positivity (CPE), though measured under various protocols (directly [87,91,101,135,143,145,200,216,241] and indirectly [141,169,201,215,241,254]), has been extensively used as a marker for sample infectivity. Furthermore, twelve studies [54,76,85,143,170,199,213,217,233,235,237,241] presented data providing LoD values for a POC tests ranging from 5.10³ (Ct = 27.3 [63]) to 10⁶ RNA copies/swab (Ct = 30) [54,76]. Noteworthy, four studies on the CLEIA method [111,150,156,206] and four studies [41,44,46,47] on in-house tests also investigated virus infectivity in correlation with either Ct values or positivity of these tests, but these were

not analyzed since they were not reporting on POC tests. Taken together, the above observations suggest that if SARS-CoV-2-infected cell culture positivity is an indicator of a patient/sample that is likely to be infectious [202,258,259], this infectivity better correlates with POC test positivity than rt-PCR positivity. As we show herein, POC test positivity corresponds better to PCR positivity for Ct < 30; thus, POC tests are more likely to detect infectious individuals than positive PCR tests.

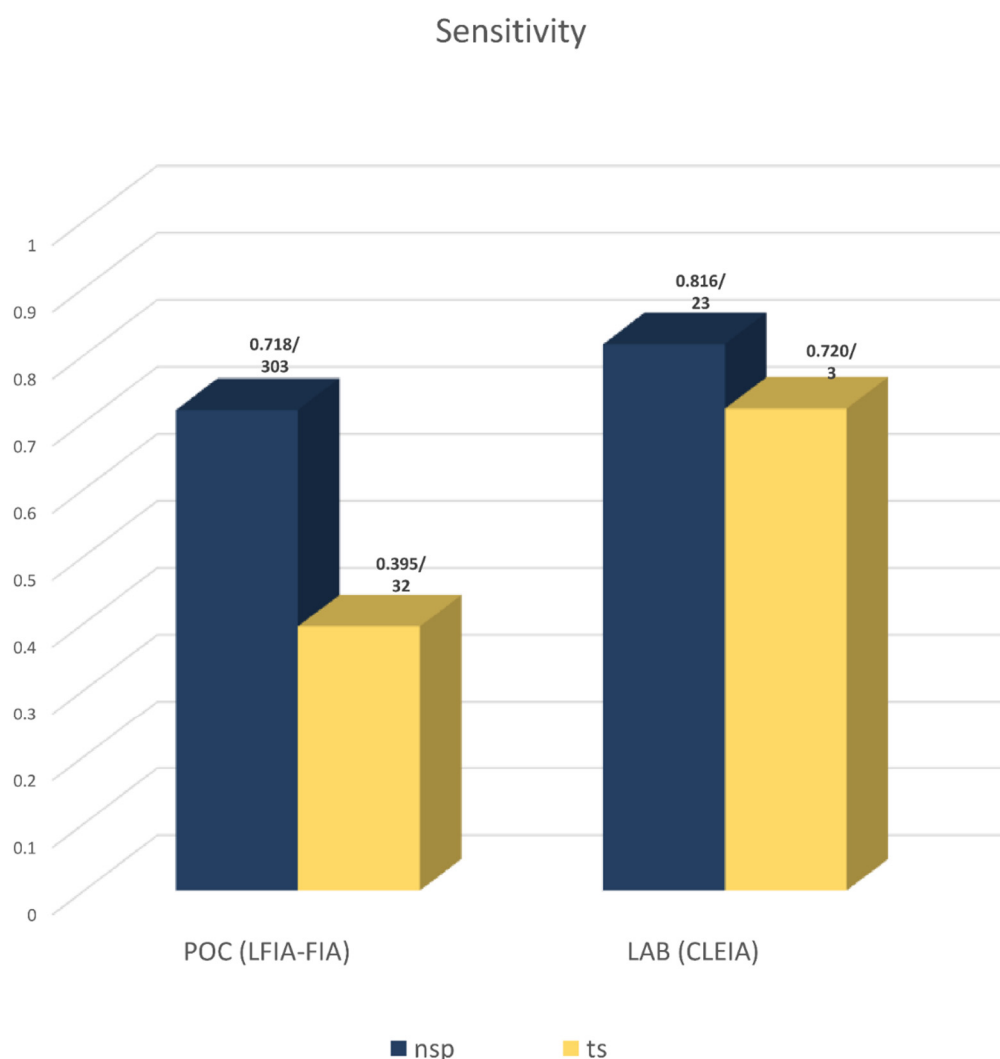


Figure 2. Performance of POC (LFIA and FIA) and laboratory (CLEIA) antigen-based methods in terms of sensitivity. All included assays in the meta-analysis use samples with Ct < 40 and test cumulatively both the nucleocapsid and Spike antigen. Numbers above the bars depict sensitivity values/number of studies included in each meta-analysis.

Additional meta-analysis showed that the sensitivity of LFIA (on NSP samples) in symptomatic patients was higher than that in asymptomatic individuals, both for Ct < 30 and Ct < 40 (symptomatic: 0.823 (95% CI: 0.765, 0.882) and 0.753 (95% CI: 0.713, 0.794)—asymptomatic: 0.665 (0.558, 0.772) and 0.561 (95% CI: 0.499, 0.622), respectively) (Table 4 and Figure 3). FIA assays seem to perform worse, but the meta-analysis estimates were based on a smaller number of studies. Specificity was very high for both LFIA and FIA methods (~99%) (Table 4).

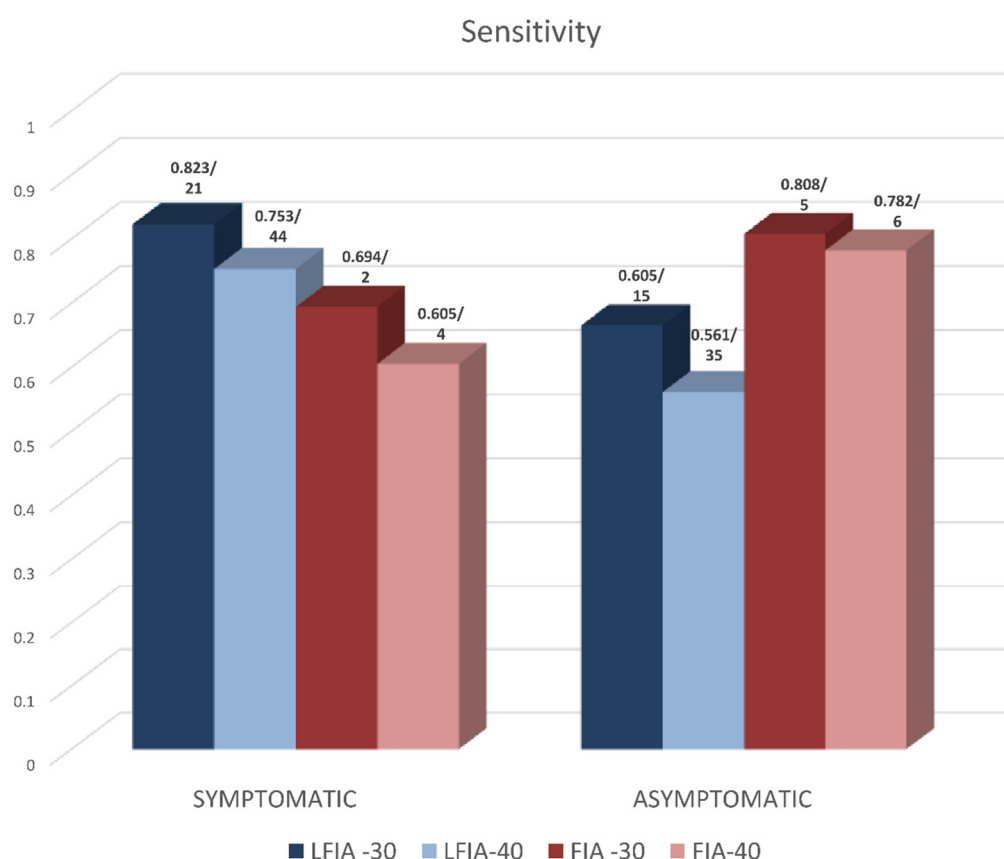


Figure 3. Performance of LFIA and FIA methods (N antigen-based) in terms of sensitivity on NSP samples in symptomatic vs. asymptomatic persons. Included assays in the meta-analysis are performed with positive samples for either Ct < 30 or Ct < 40. Numbers above the bars depict sensitivity values/number of studies included in each meta-analysis.

Table 4. Results of the meta-analysis for the different types of assays for symptomatic and asymptomatic patients. Listed information includes the pooled sensitivity and specificity along with the 95% confidence intervals. (NSP: pharyngeal, nasopharyngeal, nasal specimens, TS: throat, saliva, N: nucleocapsid protein, S: spike protein, NS: nucleocapsid and Spike proteins).

Sample	Ag	Method	Ct	Studies	Sensitivity (95% CI)	Specificity (95% CI)	Studies w/o Controls
SYMPTOMATIC INDIVIDUALS							
NSP	N	LFIA	20	1	0.976 (0.911, 1.000)	-	1
NSP	N	LFIA	30	21	0.823 (0.765, 0.882)	0.993 (0.989, 0.997)	7
NSP	N	LFIA	40	44	0.753 (0.713, 0.794)	0.992 (0.987, 0.997)	7
NSP	N	LFIA	20–30	2	0.881 (0.765, 0.996)	-	2
NSP	N	LFIA	30–40	13	0.469 (0.228, 0.709)	0.947 (0.880, 1.000)	4
NSP	N	FIA	30	2	0.694 (0.509, 0.878)	0.996 (0.993, 0.998)	0
NSP	N	FIA	40	4	0.605 (0.292, 0.918)	0.948 (0.827, 1.000)	1
NSP	N	FIA	30–40	1	0.921 (0.868, 0.973)	0.923 (0.000, 1.000)	0
TS	N	LFIA	30	2	0.669 (0.119, 1.000)	0.998 (0.994, 1.000)	0
TS	N	LFIA	40	4	0.426 (0.029, 0.823)	0.986 (0.977, 0.996)	0
TS	N	LFIA	30–40	1	0.025 (0.000, 1.000)	0.5 (0.000, 1.000)	0
TS	N	FIA	40	1	0.083 (0.000, 1.000)	-	1
NSP-TS	N	LFIA	20	2	0.957 (0.889, 1.000)	-	2
NSP-TS	N	LFIA	30	4	0.873 (0.788, 0.958)	0.998 (0.993, 1.000)	3
NSP-TS	N	LFIA	40	11	0.767 (0.695, 0.836)	0.996 (0.992, 0.999)	3
NSP-TS	N	LFIA	20–30	2	0.901 (0.795, 1.000)	-	2
NSP-TS	N	LFIA	30–40	4	0.260 (0.142, 0.378)	0.500 (0.000, 1.000)	3

ASYMPTOMATIC INDIVIDUALS							
NSP	N	LFIA	30	15	0.665 (0.558, 0.772)	0.992 (0.981, 1.000)	6
NSP	N	LFIA	40	35	0.561 (0.499, 0.622)	0.995 (0.992, 0.998)	5
NSP	N	LFIA	20–30	1	0.371 (0.270, 0.471)	-	1
NSP	N	LFIA	30–40	10	0.233 (0.061, 0.405)	0.947 (0.880, 1.000)	6
NSP	N	FIA	30	5	0.808 (0.714, 0.901)	0.997 (0.989, 1.000)	3
NSP	N	FIA	40	6	0.782 (0.614, 0.949)	0.949 (0.904, 0.995)	1
NSP	N	FIA	30–40	2	0.734 (0.253, 1.000)	0.882 (0.774, 0.991)	1
TS	N	LFIA	30	2	0.484 (0.000, 1.000)	0.995 (0.986, 1.000)	0
TS	N	LFIA	40	9	0.167 (0.034, 0.301)	0.990 (0.974, 1.000)	6
TS	N	LFIA	30–40	1	0.050 (0.000, 0.185)	0.5 (0.000, 1.000)	0
TS	N	FIA	40	1	0.166 (0.000, 1.000)	0.984 (0.941, 1.000)	0
NSP-TS	N	LFIA	30	1	0.300 (0.136, 0.464)	0.997 (0.000, 1.000)	0
NSP-TS	N	LFIA	40	5	0.481 (0.291, 0.671)	0.997 (0.995, 0.998)	1
NSP-TS	N	LFIA	30–40	1	0.050 (0.000, 0.185)	0.997 (0.000, 1.000)	0
NSP-TS	N	FIA	40	1	0.850 (0.772, 0.928)	0.984 (0.941, 1.000)	0

4. Discussion

Test-trace-isolate remains a fundamental strategy to control SARS-CoV-2 transmission. Compared to PCR methods, antigen detection tests do not require specialized laboratory equipment and are less expensive, thus allowing repeated and point-of-care testing on a wide scale [18]. Our meta-analysis, summarizing evidence from thousands of people with and without SARS-CoV-2 infection diagnosed with rt-PCR, and performing various comparisons, shows that the overall performance of AT is comparable to rt-PCR, at least in terms of specificity, with meta-analytic estimates around 99%, irrespective of the method used. Sensitivity is lower and seems to depend on viral concentration being increased if detected at lower PCR cycles (Ct values). AT are also more sensitive when used on NSP samples and in symptomatic individuals. These updated findings are in accordance with previous efforts to summarize the evidence in this field [260,261]. Current best practices in meta-analysis suggest that a frequent update should be performed, and there is active research regarding the identification of the actual time that an update is needed [262,263]. As a matter of fact, previous works include statistical methods and surveillance systems that will identify the need for an update of a published meta-analysis [264,265]. More recently, the concept of a “living” systematic review has emerged, in which the review is continuously updated, incorporating relevant new data as they become available. Such reviews may be particularly important in fields where research evidence is emerging rapidly [266,267], and clearly, the COVID-19 pandemic is a perfect example of a field where new research accumulates in an unprecedented way and an updated meta-analysis is needed.

The sensitivity of AT is good but not ideal, and thus rt-PCR remains the gold standard for diagnosis. Given the suboptimal sensitivity of antigen tests, there is a likelihood of false negative results, which should be handled depending on the clinical and epidemiological circumstances. In general, confirmation of an AT result with rt-PCR in a laboratory is necessary when the result is not consistent with clinical and epidemiological information. Given their higher sensitivity among symptomatic people and in those with higher viral load (Ct < 30), ATs are expected to perform better when used for the diagnosis of SARS-CoV-2 infection in people with symptoms, in high-risk contacts of confirmed cases or in high-risk groups as health care workers with known exposure. Moreover, the sole detection of viral RNA with rt-PCR does not seem to overlap with patients’ infectiousness. Rather, POC (rapid) antigen tests that can only detect viral loads detectable with rt-PCR at Ct values < 30 seem to more efficiently discriminate infectious SARS-CoV-2 carriers that should stay in isolation [202,255,258,259]. These findings are further supported by CDC recommendations, already posed by the end of 2020, which propose a Ct value of 33 as illustrative of contagiousness [204,268].

Proper interpretation of AT results is important not only for diagnosis but also for screening and surveillance purposes. This meta-analysis did not evaluate screening strategies that used AT. Nevertheless, it seems that AT can be used for regular screening of asymptomatic people in high-risk congregate settings, such as nursing homes, homeless shelters, detention facilities, etc., where the turnaround time of results is critical [269]. The fast identification of highly infected people in these facilities using rapid POC antigen tests will immediately inform infection prevention and control strategies and interventions, and consequently will significantly reduce onward transmission. Due to the lower sensitivity, screening in congregate high-risk settings but also mass screening may suffer from false negative results. Given the presumed direct correlation of rapid ATs' positivity with patient's infectivity, and the evidence that the effectiveness of screening depends more on frequency of testing and speed of reporting rather than on very high sensitivity [91,270], it seems that antigen tests can be used for repeated population screening.

In terms of specificity, AT performs extremely well, similarly to rt-PCR, thus minimizing the likelihood of false-positive results. However, false-positive results do occur, especially when the prevalence of SARS-CoV-2 infection in communities is low. This should be considered both in terms of diagnosis and when designing public health interventions or prevalence studies in low-prevalence settings because false positives result in a waste of resources (unnecessary isolation of cases and follow-up actions) and inaccurate estimations.

This meta-analysis is subject to the limitations of the individual studies. Bias and confounding at the study level cannot be easily addressed or corrected at the stage of meta-analysis. There are also issues that could affect the results and are usually not measured, reported, or addressed in studies that evaluate the accuracy of AT: storage and handling, reading of test results (time and interpretation), specimen collection and handling, time from specimen collection to testing, temperature of specimen, and potential cross-contamination, as was shown in the quality assessment of the research performed with the QUADAS tool.

We need to emphasize that the studies included in this meta-analysis were conducted before July 2021. Thus, data collection was completed at a time prior to the emergence of the Omicron variant and thus, the conclusions drawn from this work involve mainly the initial Wuhan strain, Alpha, Beta and Delta (to some extent) variants. A complete treatment of the question regarding the effectiveness of antigen tests against the newly emerged Omicron variant [271] would require a study of its own, but nevertheless we might be able to highlight some of the available evidence. Initially, there were concerns regarding the effectiveness of the tests [272], but the first report with the Abbott BinaxNow SARS-CoV-2 Rapid Antigen Assay provided evidence that it can be used efficiently [273]. Similar results were reported with another approved test (E25Bio, Inc., Cambridge, MA, USA, and Perkin Elmer, Waltham, MA, USA) in a comparison study of the Alpha, Gamma, Delta and Omicron variants [274], and for Panbio™ COVID-19 Ag Rapid Test [275]. Stanley and coworkers examined the analytical sensitivity of the Abbott BinaxNow, the AccessBio CareStart and LumiraDx antigen tests, and found that the level of detection was at least as good for Omicron as for the initial Wuhan strain [276]. Finally, Deerain and coworkers measured the sensitivity of ten different lateral flow devices against the omicron variant and found that the analytical sensitivities of these ten kits were similar for both the Delta and Omicron variants [277]. All in all, even though more studies are needed, the available evidence suggests that the currently used ATs can be used efficiently for detecting the Omicron variant and large discrepancies in sensitivity due to its spread are not expected.

Finally, evaluation of different testing strategies in various settings is also urgently needed [278]. Moreover, the lack of an agreed, universal, standardized protocol starting from specimen collection and handling to performing and reading the test and to the way(s) that its performance is validated (rt-PCR (genes, Ct values) or cytopathic effects of virus cultures (reference virus strain) or RNA copies, etc. [140,279]) has also been revealed

through our current systematic review and meta-analysis. Only in such uniform settings can accurate comparisons of methods and individual tests be performed in order to optimally track and manage SARS-CoV-2 infection in the global community.

Supplementary Materials: The following supporting information can be downloaded at: <https://www.mdpi.com/article/10.3390/diagnostics12061388/s1>, Table S1: The QUADAS tool; File S1: QUADAS-2 assessment results for included studies.

Author Contributions: Conceptualization: P.G.B., G.G.B. and P.I.K.; Methodology: P.I.K., G.K.N., P.G.B. and P.G.B.; Validation: G.G.B., G.K.N., P.I.K., A.T., M.P., H.M. and P.G.B.; Formal Analysis: A.T., P.G.B., G.G.B., P.I.K. and G.K.N.; Investigation: A.T., H.M., M.P., P.I.K. and G.G.B.; Resources: A.T. and G.G.B.; Data Curation: A.T., G.G.B. and P.I.K.; Writing—Original Draft Preparation: A.T. and G.G.B.; Writing—Review and Editing, P.I.K., H.M., M.P., G.K.N. and P.G.B.; Visualization: G.G.B. and P.I.K.; Supervision: G.G.B. and P.G.B. All authors have read and agreed to the published version of the manuscript.

Funding: This study received no funding.

Informed Consent Statement: Not applicable.

Conflicts of Interest: The authors declare no conflict of interest.

References

1. Estimating excess mortality due to the COVID-19 pandemic: A systematic analysis of COVID-19-related mortality, 2020–2021. *Lancet* **2022**, *399*, 1513–1536. [https://doi.org/10.1016/s0140-6736\(21\)02796-3](https://doi.org/10.1016/s0140-6736(21)02796-3).
2. IHME. Institute for Health Metrics and Evaluation—COVID-19 Results Briefing. Available online: <https://www.healthdata.org/covid/updates> (accessed on 30 March 2022).
3. Baden, L.R. El Sahly, H.M.; Essink, B.; Kotloff, K.; Frey, S.; Novak, R.; Diemert, D.; Spector, S.A.; Rouphael, N.; Creech, C.B.; et al. Efficacy and Safety of the mRNA-1273 SARS-CoV-2 Vaccine. *N. Engl. J. Med.* **2021**, *384*, 403–416. <https://doi.org/10.1056/NEJMoa2035389>.
4. Heath, P.T.; Galiza, E.P.; Baxter, D.N.; Boffito, M.; Browne, D.; Burns, F.; Chadwick, D.R.; Clark, R.; Cosgrove, C.; Galloway, J.; et al. Safety and Efficacy of NVX-CoV2373 Covid-19 Vaccine. *N. Engl. J. Med.* **2021**, *385*, 1172–1183. <https://doi.org/10.1056/NEJMoa2107659>.
5. Hyams, C.; Marlow, R.; Maseko, Z.; King, J.; Ward, L.; Fox, K.; Heath, R.; Tuner, A.; Friedrich, Z.; Morrison, L.; et al. Effectiveness of BNT162b2 and ChAdOx1 nCoV-19 COVID-19 vaccination at preventing hospitalisations in people aged at least 80 years: A test-negative, case-control study. *Lancet Infect. Dis.* **2021**, *21*, 1539–1548. [https://doi.org/10.1016/s1473-3099\(21\)00330-3](https://doi.org/10.1016/s1473-3099(21)00330-3).
6. Polack, F.P.; Thomas, S.J.; Kitchin, N.; Absalon, J.; Gurtman, A.; Lockhart, S.; Perez, J.L.; Pérez Marc, G.; Moreira, E.D.; Zerbini, C.; et al. Safety and Efficacy of the BNT162b2 mRNA Covid-19 Vaccine. *N. Engl. J. Med.* **2020**, *383*, 2603–2615. <https://doi.org/10.1056/NEJMoa2034577>.
7. Voysey, M.; Clemens, S.A.C.; Madhi, S.A.; Weckx, L.Y.; Folegatti, P.M.; Aley, P.K.; Angus, B.; Baillie, V.L.; Barnabas, S.L.; Bhorat, Q.E.; et al. Safety and efficacy of the ChAdOx1 nCoV-19 vaccine (AZD1222) against SARS-CoV-2: An interim analysis of four randomised controlled trials in Brazil, South Africa, and the UK. *Lancet* **2021**, *397*, 99–111. [https://doi.org/10.1016/s0140-6736\(20\)32661-1](https://doi.org/10.1016/s0140-6736(20)32661-1).
8. Taylor, C.A.; Whitaker, M.; Anglin, O.; Milucky, J.; Patel, K.; Pham, H.; Chai, S.J.; Alden, N.B.; Yousey-Hindes, K.; Anderson, E.J.; et al. COVID-19-Associated Hospitalizations Among Adults During SARS-CoV-2 Delta and Omicron Variant Predominance, by Race/Ethnicity and Vaccination Status—COVID-NET, 14 States, July 2021–January 2022. *MMWR Morb. Mortal Wkly. Rep.* **2022**, *71*, 466–473. <https://doi.org/10.15585/mmwr.mm7112e2>.
9. Chemaitelly, H.; Ayoub, H.H.; AlMukdad, S.; Coyle, P.; Tang, P.; Yassine, H.M.; Al-Khatib, H.A.; Smatti, M.K.; Hasan, M.R.; Al-Kanaani, Z.; et al. Duration of mRNA vaccine protection against SARS-CoV-2 Omicron BA.1 and BA.2 subvariants in Qatar. *medRxiv* **2022**. <https://doi.org/10.1101/2022.03.13.22272308>.
10. Flaxman, S.; Mishra, S.; Gandy, A.; Unwin, H.J.T.; Mellan, T.A.; Coupland, H.; Whittaker, C.; Zhu, H.; Berah, T.; Eaton, J.W.; et al. Estimating the effects of non-pharmaceutical interventions on COVID-19 in Europe. *Nature* **2020**, *584*, 257–261. <https://doi.org/10.1038/s41586-020-2405-7>.
11. Fuller, J.A.; Hakim, A.; Victory, K.R.; Date, K.; Lynch, M.; Dahl, B.; Henao, O. Mitigation Policies and COVID-19-Associated Mortality—37 European Countries, 23 January–30 June 2020. *MMWR Morb. Mortal. Wkly. Rep.* **2021**, *70*, 58–62. <https://doi.org/10.15585/mmwr.mm7002e4>.
12. Piovani, D.; Christodoulou, M.N.; Hadjidemetriou, A.; Pantavou, K.; Zaza, P.; Bagos, P.G.; Bonovas, S.; Nikolopoulos, G.K. Effect of early application of social distancing interventions on COVID-19 mortality over the first pandemic wave: An analysis of longitudinal data from 37 countries. *J. Infect.* **2021**, *82*, 133–142. <https://doi.org/10.1016/j.jinf.2020.11.033>.
13. ECDC. European Centre for Disease Prevention and Control. COVID-19 Testing Strategies and Objectives. Available online: <https://www.ecdc.europa.eu/en/publications-data/covid-19-testing-strategies-and-objectives> (accessed on 30 March 2022).

14. TheWhiteHouse. National COVID-19 Preparedness Plan. Available online: <https://www.whitehouse.gov/covidplan/> (accessed on 3 March 2022).
15. Chan, J.F.; Yip, C.C.; To, K.K.; Tang, T.H.; Wong, S.C.; Leung, K.H.; Fung, A.Y.; Ng, A.C.; Zou, Z.; Tsoi, H.W.; et al. Improved Molecular Diagnosis of COVID-19 by the Novel, Highly Sensitive and Specific COVID-19-RdRp/Hel Real-Time Reverse Transcription-PCR Assay Validated In Vitro and with Clinical Specimens. *J. Clin. Microbiol.* **2020**, *58*, e00310-20. <https://doi.org/10.1128/jcm.00310-20>.
16. Corman, V.M.; Landt, O.; Kaiser, M.; Molenkamp, R.; Meijer, A.; Chu, D.K.; Bleicker, T.; Brünink, S.; Schneider, J.; Schmidt, M.L.; et al. Detection of 2019 novel coronavirus (2019-nCoV) by real-time RT-PCR. *Euro Surveill.* **2020**, *25*, 2000045. <https://doi.org/10.2807/1560-7917.Es.2020.25.3.2000045>.
17. Reusken, C.; Broberg, E.K.; Haagmans, B.; Meijer, A.; Corman, V.M.; Papa, A.; Charrel, R.; Drosten, C.; Koopmans, M.; Leitmeyer, K.; et al. Laboratory readiness and response for novel coronavirus (2019-nCoV) in expert laboratories in 30 EU/EEA countries, January 2020. *Euro Surveill.* **2020**, *25*, 2000082. <https://doi.org/10.2807/1560-7917.Es.2020.25.6.2000082>.
18. Mina, M.J.; Parker, R.; Larremore, D.B. Rethinking Covid-19 Test Sensitivity—A Strategy for Containment. *N. Engl. J. Med.* **2020**, *383*, e120. <https://doi.org/10.1056/NEJMp2025631>.
19. Peto, T. COVID-19: Rapid antigen detection for SARS-CoV-2 by lateral flow assay: A national systematic evaluation of sensitivity and specificity for mass-testing. *EClinicalMedicine* **2021**, *36*, 100924. <https://doi.org/10.1016/j.eclinm.2021.100924>.
20. Rai, P.; Kumar, B.K.; Deekshit, V.K.; Karunasagar, I.; Karunasagar, I. Detection technologies and recent developments in the diagnosis of COVID-19 infection. *Appl. Microbiol. Biotechnol.* **2021**, *105*, 441–455. <https://doi.org/10.1007/s00253-020-11061-5>.
21. Porte, L.; Legarraga, P.; Vollrath, V.; Aguilera, X.; Munita, J.M.; Araos, R.; Pizarro, G.; Vial, P.; Iruretagoyena, M.; Dittrich, S.; et al. Evaluation of a novel antigen-based rapid detection test for the diagnosis of SARS-CoV-2 in respiratory samples. *Int. J. Infect. Dis.* **2020**, *99*, 328–333. <https://doi.org/10.1016/j.ijid.2020.05.098>.
22. Moher, D.; Liberati, A.; Tetzlaff, J.; Altman, D.G. Preferred reporting items for systematic reviews and meta-analyses: The PRISMA statement. *PLoS Med.* **2009**, *6*, e1000097. <https://doi.org/10.1371/journal.pmed.1000097>.
23. Forero, D.A.; Lopez-Leon, S.; González-Giraldo, Y.; Bagos, P.G. Ten simple rules for carrying out and writing meta-analyses. *PLoS Comput. Biol.* **2019**, *15*, e1006922. <https://doi.org/10.1371/journal.pcbi.1006922>.
24. Hopewell, S.; McDonald, S.; Clarke, M.; Egger, M. Grey literature in meta-analyses of randomized trials of health care interventions. *Cochrane Database Syst. Rev.* **2007**, *2007*, Mr000010. <https://doi.org/10.1002/14651858.MR000010.pub3>.
25. World Health Organization (WHO). Coronavirus Disease (COVID-19) Technical Guidance: Laboratory Testing for 2019-nCoV in Humans. Available online: <https://www.who.int/emergencies/diseases/novel-coronavirus-2019/technical-guidance/laboratory-guidance/> (accessed on 17 March 2022).
26. Centers for Disease Control and Prevention (CDC). Information for Laboratories about Coronavirus (COVID-19). Available online: <https://www.cdc.gov/coronavirus/2019-ncov/lab/index.html> (accessed on 13 March 2022).
27. ECDC. European Centre for Disease Prevention and Control. Novel Coronavirus Disease 2019 (COVID-19) Pandemic: Increased Transmission in the EU/EEA and the UK—Sixth Update—12 March 2020. Available online: <https://www.ecdc.europa.eu/sites/default/files/documents/RRA-sixth-update-Outbreak-of-novel-coronavirus-disease-2019-COVID-19.pdf> (accessed on 12 March 2022).
28. Whiting, P.F.; Rutjes, A.W.; Westwood, M.E.; Mallett, S.; Deeks, J.J.; Reitsma, J.B.; Leeflang, M.M.; Sterne, J.A.; Bossuyt, P.M. QUADAS-2: A revised tool for the quality assessment of diagnostic accuracy studies. *Ann. Intern. Med.* **2011**, *155*, 529–536. <https://doi.org/10.7326/0003-4819-155-8-201110180-00009>.
29. Van Houwelingen, H.C.; Zwinderman, K.H.; Stijnen, T. A bivariate approach to meta-analysis. *Stat. Med.* **1993**, *12*, 2273–2284. <https://doi.org/10.1002/sim.4780122405>.
30. Harbord, R.M.; Deeks, J.J.; Egger, M.; Whiting, P.; Sterne, J.A. A unification of models for meta-analysis of diagnostic accuracy studies. *Biostatistics* **2007**, *8*, 239–251. <https://doi.org/10.1093/biostatistics/kxl004>.
31. Higgins, J.P.; Whitehead, A. Borrowing strength from external trials in a meta-analysis. *Stat. Med.* **1996**, *15*, 2733–2749.
32. Begg, C.B.; Mazumdar, M. Operating characteristics of a rank correlation test for publication bias. *Biometrics* **1994**, *50*, 1088–1101.
33. Egger, M.; Davey Smith, G.; Schneider, M.; Minder, C. Bias in meta-analysis detected by a simple, graphical test. *BMJ* **1997**, *315*, 629–634. <https://doi.org/10.1136/bmj.315.7109.629>.
34. StataCorp. *Stata Statistical Software: Release 13*; Stata Press: College Station, TX, USA, 2013.
35. White, I.R. Multivariate random-effects meta-regression: Updates to mvmeta. *Stata J.* **2011**, *11*, 255–270.
36. Chavan, S.; Mangalaparthy, K.K.; Singh, S.; Renuse, S.; Vanderboom, P.M.; Madugundu, A.K.; Budhraj, R.; McAulay, K.; Grys, T.E.; Rule, A.D.; et al. Mass Spectrometric Analysis of Urine from COVID-19 Patients for Detection of SARS-CoV-2 Viral Antigen and to Study Host Response. *J. Proteome Res.* **2021**, *20*, 3404–3413. <https://doi.org/10.1021/acs.jproteome.1c00391>.
37. Saadi, J.; Oueslati, S.; Bellanger, L.; Gallais, F.; Dortet, L.; Roque-Afonso, A.M.; Junot, C.; Naas, T.; Fenaille, F.; Becher, F. Quantitative Assessment of SARS-CoV-2 Virus in Nasopharyngeal Swabs Stored in Transport Medium by a Straightforward LC-MS/MS Assay Targeting Nucleocapsid, Membrane, and Spike Proteins. *J. Proteome Res.* **2021**, *20*, 1434–1443. <https://doi.org/10.1021/acs.jproteome.0c00887>.
38. Shao, W.; Shurin, M.R.; Wheeler, S.E.; He, X.; Star, A. Rapid Detection of SARS-CoV-2 Antigens Using High-Purity Semiconducting Single-Walled Carbon Nanotube-Based Field-Effect Transistors. *ACS Appl. Mater. Interfaces* **2021**, *13*, 10321–10327. <https://doi.org/10.1021/acsami.0c22589>.

39. Guo, K.; Wustoni, S.; Koklu, A.; Díaz-Galicia, E.; Moser, M.; Hama, A.; Alqahtani, A.A.; Ahmad, A.N.; Alhamlan, F.S.; Shuaib, M.; et al. Rapid single-molecule detection of COVID-19 and MERS antigens via nanobody-functionalized organic electrochemical transistors. *Nat. Biomed. Eng.* **2021**, *5*, 666–677. <https://doi.org/10.1038/s41551-021-00734-9>.
40. Eissa, S.; Alhadrami, H.A.; Al-Mozaini, M.; Hassan, A.M.; Zourob, M. Voltammetric-based immunosensor for the detection of SARS-CoV-2 nucleocapsid antigen. *Mikrochim. Acta* **2021**, *188*, 199. <https://doi.org/10.1007/s00604-021-04867-1>.
41. Funabashi, R.; Miyakawa, K.; Yamaoka, Y.; Yoshimura, S.; Yamane, S.; Jeremiah, S.S.; Shimizu, K.; Ozawa, H.; Kawakami, C.; Usuku, S.; et al. Development of highly sensitive and rapid antigen detection assay for diagnosis of COVID-19 utilizing optical waveguide immunosensor. *J. Mol. Cell Biol.* **2021**, *13*, 763–766. <https://doi.org/10.1093/jmcb/mjab037>.
42. Huang, J.; Wen, J.; Zhou, M.; Ni, S.; Le, W.; Chen, G.; Wei, L.; Zeng, Y.; Qi, D.; Pan, M.; et al. On-Site Detection of SARS-CoV-2 Antigen by Deep Learning-Based Surface-Enhanced Raman Spectroscopy and Its Biochemical Foundations. *Anal. Chem.* **2021**, *93*, 9174–9182. <https://doi.org/10.1021/acs.analchem.1c01061>.
43. Ehsan, M.A.; Khan, S.A.; Rehman, A. Screen-Printed Graphene/Carbon Electrodes on Paper Substrates as Impedance Sensors for Detection of Coronavirus in Nasopharyngeal Fluid Samples. *Diagnostics* **2021**, *11*, 1030. <https://doi.org/10.3390/diagnostics11061030>.
44. Renuse, S.; Vanderboom, P.M.; Maus, A.D.; Kemp, J.V.; Gurtner, K.M.; Madugundu, A.K.; Chavan, S.; Peterson, J.A.; Madden, B.J.; Mangalparthi, K.K.; et al. A mass spectrometry-based targeted assay for detection of SARS-CoV-2 antigen from clinical specimens. *EBioMedicine* **2021**, *69*, 103465. <https://doi.org/10.1016/j.ebiom.2021.103465>.
45. Della Ventura, B.; Cennamo, M.; Minopoli, A.; Campanile, R.; Bolletti Censi, S.; Terracciano, D.; Portella, G.; Velotta, R. Colorimetric Test for Fast Detection of SARS-CoV-2 in Nasal and Throat Swabs. *medRxiv* **2020**. <https://doi.org/10.1101/2020.08.15.20175489>.
46. Singh, N.K.; Ray, P.; Carlin, A.F.; Magallanes, C.; Morgan, S.C.; Laurent, L.C.; Aronoff-Spencer, E.S.; Hall, D.A. Hitting the diagnostic sweet spot: Point-of-care SARS-CoV-2 salivary antigen testing with an off-the-shelf glucometer. *medRxiv* **2020**. <https://doi.org/10.1101/2020.09.24.20200394>.
47. Kurtulmus, M.S.; Kazezoglu, C.; Cakiroglu, B.; Yilmaz, H.; Guner, A.E. The urine foaming test in COVID-19 as a useful tool in diagnosis, prognosis and follow-up: Preliminary results. *North Clin. Istanbul* **2020**, *7*, 534–540. <https://doi.org/10.14744/nci.2020.42027>.
48. Mak, G.C.; Lau, S.S.; Wong, K.K.; Chow, N.L.; Lau, C.S.; Lam, E.T.; Chan, R.C.; Tsang, D.N. Analytical sensitivity and clinical sensitivity of the three rapid antigen detection kits for detection of SARS-CoV-2 virus. *J. Clin. Virol.* **2020**, *133*, 104684. <https://doi.org/10.1016/j.jcv.2020.104684>.
49. Linares, M.; Pérez-Tanoira, R.; Carrero, A.; Romanyk, J.; Pérez-García, F.; Gómez-Herruz, P.; Arroyo, T.; Cuadros, J. Panbio antigen rapid test is reliable to diagnose SARS-CoV-2 infection in the first 7 days after the onset of symptoms. *J. Clin. Virol.* **2020**, *133*, 104659. <https://doi.org/10.1016/j.jcv.2020.104659>.
50. Gupta, A.; Khurana, S.; Das, R.; Srigyan, D.; Singh, A.; Mittal, A.; Singh, P.; Soneja, M.; Kumar, A.; Singh, A.K.; et al. Rapid chromatographic immunoassay-based evaluation of COVID-19: A cross-sectional, diagnostic test accuracy study & its implications for COVID-19 management in India. *Indian J. Med. Res.* **2021**, *153*, 126. https://doi.org/10.4103/ijmr.IJMR_3305_20.
51. Fenollar, F.; Bouam, A.; Ballouche, M.; Fuster, L.; Prudent, E.; Colson, P.; Tissot-Dupont, H.; Million, M.; Drancourt, M.; Raoult, D.; et al. Evaluation of the Panbio COVID-19 Rapid Antigen Detection Test Device for the Screening of Patients with COVID-19. *J. Clin. Microbiol.* **2021**, *59*, e02589-20. <https://doi.org/10.1128/jcm.02589-20>.
52. Nalumansi, A.; Lutalo, T.; Kayiwa, J.; Watera, C.; Balinandi, S.; Kiconco, J.; Nakaseegu, J.; Olara, D.; Odwilo, E.; Serwanga, J.; et al. Field evaluation of the performance of a SARS-CoV-2 antigen rapid diagnostic test in Uganda using nasopharyngeal samples. *Int. J. Infect. Dis.* **2021**, *104*, 282–286. <https://doi.org/10.1016/j.ijid.2020.10.073>.
53. Parada-Ricart, E.; Gomez-Bertomeu, F.; Picó-Plana, E.; Olona-Cabases, M. Usefulness of the antigen test for diagnosing SARS-CoV-2 infection in patients with and without symptoms. *Enferm. Infecc. Microbiol. Clin.* **2021**, *39*, 357–358. <https://doi.org/10.1016/j.eimce.2021.05.003>.
54. Lee, J.H.; Choi, M.; Jung, Y.; Lee, S.K.; Lee, C.S.; Kim, J.; Kim, J.; Kim, N.H.; Kim, B.T.; Kim, H.G. A novel rapid detection for SARS-CoV-2 spike 1 antigens using human angiotensin converting enzyme 2 (ACE2). *Biosens. Bioelectron.* **2021**, *171*, 112715. <https://doi.org/10.1016/j.bios.2020.112715>.
55. Cerutti, F.; Burdino, E.; Milia, M.G.; Allice, T.; Gregori, G.; Bruzzzone, B.; Ghisetti, V. Urgent need of rapid tests for SARS CoV-2 antigen detection: Evaluation of the SD-Biosensor antigen test for SARS-CoV-2. *J. Clin. Virol.* **2020**, *132*, 104654. <https://doi.org/10.1016/j.jcv.2020.104654>.
56. Diao, B.; Wen, K.; Zhang, J.; Chen, J.; Han, C.; Chen, Y.; Wang, S.; Deng, G.; Zhou, H.; Wu, Y. Accuracy of a nucleocapsid protein antigen rapid test in the diagnosis of SARS-CoV-2 infection. *Clin. Microbiol. Infect.* **2021**, *27*, 289.e281–289.e284. <https://doi.org/10.1016/j.cmi.2020.09.057>.
57. Young, S.; Taylor, S.N.; Cammarata, C.L.; Varnado, K.G.; Roger-Dalbert, C.; Montano, A.; Griego-Fullbright, C.; Burgard, C.; Fernandez, C.; Eckert, K.; et al. Clinical Evaluation of BD Veritor SARS-CoV-2 Point-of-Care Test Performance Compared to PCR-Based Testing and versus the Sofia 2 SARS Antigen Point-of-Care Test. *J. Clin. Microbiol.* **2020**, *59*, e02338-20. <https://doi.org/10.1128/jcm.02338-20>.
58. Liotti, F.M.; Menchinelli, G.; Lalle, E.; Palucci, I.; Marchetti, S.; Colavita, F.; La Sorda, M.; Sberna, G.; Bordini, L.; Sanguinetti, M.; et al. Performance of a novel diagnostic assay for rapid SARS-CoV-2 antigen detection in nasopharynx samples. *Clin. Microbiol. Infect.* **2021**, *27*, 487–488. <https://doi.org/10.1016/j.cmi.2020.09.030>.

59. Ogawa, T.; Fukumori, T.; Nishihara, Y.; Sekine, T.; Okuda, N.; Nishimura, T.; Fujikura, H.; Hirai, N.; Imakita, N.; Kasahara, K. Another false-positive problem for a SARS-CoV-2 antigen test in Japan. *J. Clin. Virol.* **2020**, *131*, 104612. <https://doi.org/10.1016/j.jcv.2020.104612>.
60. Hirotsu, Y.; Maejima, M.; Shibusawa, M.; Nagakubo, Y.; Hosaka, K.; Amemiya, K.; Sueki, H.; Hayakawa, M.; Mochizuki, H.; Tsutsui, T.; et al. Comparison of automated SARS-CoV-2 antigen test for COVID-19 infection with quantitative RT-PCR using 313 nasopharyngeal swabs, including from seven serially followed patients. *Int. J. Infect. Dis.* **2020**, *99*, 397–402. <https://doi.org/10.1016/j.ijid.2020.08.029>.
61. Nagura-Ikeda, M.; Imai, K.; Tabata, S.; Miyoshi, K.; Murahara, N.; Mizuno, T.; Horiuchi, M.; Kato, K.; Imoto, Y.; Iwata, M.; et al. Clinical Evaluation of Self-Collected Saliva by Quantitative Reverse Transcription-PCR (RT-qPCR), Direct RT-qPCR, Reverse Transcription-Loop-Mediated Isothermal Amplification, and a Rapid Antigen Test To Diagnose COVID-19. *J. Clin. Microbiol.* **2020**, *58*, e01438-20. <https://doi.org/10.1128/jcm.01438-20>.
62. Mak, G.C.; Cheng, P.K.; Lau, S.S.; Wong, K.K.; Lau, C.S.; Lam, E.T.; Chan, R.C.; Tsang, D.N. Evaluation of rapid antigen test for detection of SARS-CoV-2 virus. *J. Clin. Virol.* **2020**, *129*, 104500. <https://doi.org/10.1016/j.jcv.2020.104500>.
63. Mertens, P.; De Vos, N.; Martiny, D.; Jassoy, C.; Mirazimi, A.; Cuypers, L.; Van den Wijngaert, S.; Monteil, V.; Melin, P.; Stoffels, K.; et al. Development and Potential Usefulness of the COVID-19 Ag Respi-Strip Diagnostic Assay in a Pandemic Context. *Front. Med.* **2020**, *7*, 225. <https://doi.org/10.3389/fmed.2020.00225>.
64. Blairon, L.; Wilmet, A.; Beukinga, I.; Tré-Hardy, M. Implementation of rapid SARS-CoV-2 antigenic testing in a laboratory without access to molecular methods: Experiences of a general hospital. *J. Clin. Virol.* **2020**, *129*, 104472. <https://doi.org/10.1016/j.jcv.2020.104472>.
65. Scohy, A.; Anantharajah, A.; Bodéus, M.; Kabamba-Mukadi, B.; Verroken, A.; Rodriguez-Villalobos, H. Low performance of rapid antigen detection test as frontline testing for COVID-19 diagnosis. *J. Clin. Virol.* **2020**, *129*, 104455. <https://doi.org/10.1016/j.jcv.2020.104455>.
66. Lambert-Niclot, S.; Cuffel, A.; Le Pape, S.; Vauloup-Fellous, C.; Morand-Joubert, L.; Roque-Afonso, A.M.; Le Goff, J.; Delaugerre, C. Evaluation of a Rapid Diagnostic Assay for Detection of SARS-CoV-2 Antigen in Nasopharyngeal Swabs. *J. Clin. Microbiol.* **2020**, *58*, e00977-20. <https://doi.org/10.1128/jcm.00977-20>.
67. Diao, B.; Wen, K.; Chen, J.; Liu, Y.; Yuan, Z.; Han, C.; Chen, J.; Pan, Y.; Chen, L.; Dan, Y.; et al. Diagnosis of Acute Respiratory Syndrome Coronavirus 2 Infection by Detection of Nucleocapsid Protein. *medRxiv* **2020**. <https://doi.org/10.1101/2020.03.07.20032524>.
68. Beck, E.T.; Paar, W.; Fojut, L.; Serwe, J.; Jahnke, R.R. Comparison of the Quidel Sofia SARS FIA Test to the Hologic Aptima SARS-CoV-2 TMA Test for Diagnosis of COVID-19 in Symptomatic Outpatients. *J. Clin. Microbiol.* **2021**, *59*, e02727-20. <https://doi.org/10.1128/jcm.02727-20>.
69. Krüttgen, A.; Cornelissen, C.G.; Dreher, M.; Hornef, M.W.; Imöhl, M.; Kleines, M. Comparison of the SARS-CoV-2 Rapid antigen test to the real star Sars-CoV-2 RT PCR kit. *J. Virol. Methods* **2021**, *288*, 114024. <https://doi.org/10.1016/j.jviromet.2020.114024>.
70. Albert, E.; Torres, I.; Bueno, F.; Huntley, D.; Molla, E.; Fernández-Fuentes, M.; Martínez, M.; Poujois, S.; Forqué, L.; Valdivia, A.; et al. Field evaluation of a rapid antigen test (Panbio™ COVID-19 Ag Rapid Test Device) for COVID-19 diagnosis in primary healthcare centres. *Clin. Microbiol. Infect.* **2021**, *27*, 472.e477–472.e410. <https://doi.org/10.1016/j.cmi.2020.11.004>.
71. Chaimayo, C.; Kaewnaphan, B.; Tanlieng, N.; Athipanyasilp, N.; Sirijatuphat, R.; Chayakulkeeree, M.; Angkasekwinai, N.; Sutthent, R.; Puangpunngam, N.; Tharmviboonsri, T.; et al. Rapid SARS-CoV-2 antigen detection assay in comparison with real-time RT-PCR assay for laboratory diagnosis of COVID-19 in Thailand. *Virol. J.* **2020**, *17*, 177. <https://doi.org/10.1186/s12985-020-01452-5>.
72. Lanser, L.; Bellmann-Weiler, R.; Öttl, K.W.; Huber, L.; Griesmacher, A.; Theurl, I.; Weiss, G. Evaluating the clinical utility and sensitivity of SARS-CoV-2 antigen testing in relation to RT-PCR Ct values. *Infection* **2021**, *49*, 555–557. <https://doi.org/10.1007/s15010-020-01542-0>.
73. Gremmels, H.; Winkel, B.M.F.; Schuurman, R.; Rosingh, A.; Rigter, N.A.M.; Rodriguez, O.; Ubijaan, J.; Wensing, A.M.J.; Bonten, M.J.M.; Hofstra, L.M. Real-life validation of the Panbio™ COVID-19 antigen rapid test (Abbott) in community-dwelling subjects with symptoms of potential SARS-CoV-2 infection. *EClinicalMedicine* **2021**, *31*, 100677. <https://doi.org/10.1016/j.eclinm.2020.100677>.
74. Dřevínek, P.; Hurych, J.; Kepka, Z.; Briksi, A.; Kulich, M.; Zajac, M.; Hubáček, P. The sensitivity of SARS-CoV-2 antigen tests in the view of large-scale testing. *Epidemiol. Mikrobiol. Imunol.* **2021**, *70*, 156–160.
75. Schwob, J.M.; Miauton, A.; Petrovic, D.; Perdrix, J.; Senn, N.; Jatton, K.; Onya, O.; Maillard, A.; Minghelli, G.; Cornuz, J.; et al. Antigen rapid tests, nasopharyngeal PCR and saliva PCR to detect SARS-CoV-2: A prospective comparative clinical trial. *medRxiv* **2020**. <https://doi.org/10.1101/2020.11.23.20237057>.
76. Corman, V.M.; Haage, V.C.; Bleicker, T.; Schmidt, M.L.; Mühlemann, B.; Zuchowski, M.; Jo, W.K.; Tscheak, P.; Möncke-Buchner, E.; Müller, M.A.; et al. Comparison of seven commercial SARS-CoV-2 rapid point-of-care antigen tests: A single-centre laboratory evaluation study. *Lancet Microbe* **2021**, *2*, e311–e319. [https://doi.org/10.1016/s2666-5247\(21\)00056-2](https://doi.org/10.1016/s2666-5247(21)00056-2).
77. Abdulrahman, A.; Mustafa, F.; AlAwadhi, A.I.; Alansari, Q.; AlAlawi, B.; AlQahtani, M. Comparison of SARS-COV-2 nasal antigen test to nasopharyngeal RT-PCR in mildly symptomatic patients. *medRxiv* **2020**. <https://doi.org/10.1101/2020.11.10.20228973>.

78. Yokota, I.; Sakurazawa, T.; Sugita, J.; Iwasaki, S.; Yasuda, K.; Yamashita, N.; Fujisawa, S.; Nishida, M.; Konno, S.; Teshima, T. Performance of Qualitative and Quantitative Antigen Tests for SARS-CoV-2 Using Saliva. *Infect. Dis. Rep.* **2021**, *13*, 742–747. <https://doi.org/10.3390/idr13030069>.
79. Nash, B.; Badea, A.; Reddy, A.; Bosch, M.; Salcedo, N.; Gomez, A.R.; Versiani, A.; Dutra Silva, G.C.; Lopes dos Santos, T.M.I.; Milhim, B.H.G.A.; et al. Validating and modeling the impact of high-frequency rapid antigen screening on COVID-19 spread and outcomes. *medRxiv* **2021**. <https://doi.org/10.1101/2020.09.01.20184713>.
80. Van der Moeren, N.; Zwart, V.F.; Lodder, E.B.; van den Bijllaardt, W.; van Esch, H.R.J.M.; Stohr, J.J.J.M.; Pot, J.; Welschen, I.; van Mechelen, P.M.F.; Pas, S.D.; et al. Performance evaluation of a Sars-Cov-2 Rapid antigen test: Test performance in the community in the Netherlands. *medRxiv* **2020**. <https://doi.org/10.1101/2020.10.19.20215202>.
81. Porte, L.; Legarraga, P.; Iruretagoyena, M.; Vollrath, V.; Pizarro, G.; Munita, J.M.; Araos, R.; Weitzel, T. Rapid SARS-CoV-2 antigen detection by immunofluorescence—A new tool to detect infectivity. *medRxiv* **2020**. <https://doi.org/10.1101/2020.10.04.20206466>.
82. Krüger, L.J.; Gaedert, M.; Köppel, L.; Brümmer, L.E.; Gottschalk, C.; Miranda, I.B.; Schnitzler, P.; Kräusslich, H.G.; Lindner, A.K.; Nikolai, O.; et al. Evaluation of the accuracy, ease of use and limit of detection of novel, rapid, antigen-detecting point-of-care diagnostics for SARS-CoV-2. *medRxiv* **2020**. <https://doi.org/10.1101/2020.10.01.20203836>.
83. Ventura, B.D.; Cennamo, M.; Minopoli, A.; Campanile, R.; Censi, S.B.; Terracciano, D.; Portella, G.; Velotta, R. Colorimetric Test for Fast Detection of SARS-CoV-2 in Nasal and Throat Swabs. *ACS Sens.* **2020**, *5*, 3043–3048. <https://doi.org/10.1021/acssens.0c01742>.
84. Herrera, V.; Hsu, V.; Adewale, A.; Johnson, L.; Hendrix, T.; Kuhlman, J.; Finkler, N. Testing Healthcare Workers Exposed to COVID19 using Rapid Antigen Detection. *medRxiv* **2020**. <https://doi.org/10.1101/2020.08.12.20172726>.
85. Pickering, S.; Batra, R.; Merrick, B.; Snell, L.B.; Nebbia, G.; Douthwaite, S.; Reid, F.; Patel, A.; Kia Ik, M.T.; Patel, B.; et al. Comparative performance of SARS-CoV-2 lateral flow antigen tests and association with detection of infectious virus in clinical specimens: A single-centre laboratory evaluation study. *Lancet Microbe* **2021**, *2*, e461–e471. [https://doi.org/10.1016/s2666-5247\(21\)00143-9](https://doi.org/10.1016/s2666-5247(21)00143-9).
86. Harmon, K.; de St Maurice, A.M.; Brady, A.C.; Swaminathan, S.; Aukerman, D.F.; Rueda, M.A.; Terrell, K.; Cohen, R.P.; Gamradt, S.C.; Henry, S.D.; et al. Surveillance testing for SARS-COV-2 infection in an asymptomatic athlete population: A prospective cohort study with 123 362 tests and 23 463 paired RT-PCR/antigen samples. *BMJ Open Sport Exerc. Med.* **2021**, *7*, e001137. <https://doi.org/10.1136/bmjsem-2021-001137>.
87. Korenkov, M.; Poopalasingam, N.; Madler, M.; Vanshylla, K.; Eggeling, R.; Wirtz, M.; Fish, I.; Dewald, F.; Gieselmann, L.; Lehmann, C.; et al. Evaluation of a Rapid Antigen Test to Detect SARS-CoV-2 Infection and Identify Potentially Infectious Individuals. *J. Clin. Microbiol.* **2021**, *59*, e0089621. <https://doi.org/10.1128/jcm.00896-21>.
88. Seynaeve, Y.; Heylen, J.; Fontaine, C.; Maclot, F.; Meex, C.; Diep, A.N.; Donneau, A.F.; Hayette, M.P.; Descy, J. Evaluation of Two Rapid Antigen Tests for the Detection of SARS-CoV-2 in Nasopharyngeal Swabs. *J. Clin. Med.* **2021**, *10*, 2774. <https://doi.org/10.3390/jcm10132774>.
89. Di Domenico, M.; De Rosa, A.; Di Gaudio, F.; Internicola, P.; Bettini, C.; Salzano, N.; Castrianni, D.; Marotta, A.; Boccellino, M. Diagnostic Accuracy of a New Antigen Test for SARS-CoV-2 Detection. *Int. J. Environ. Res. Public Health* **2021**, *18*, 6310. <https://doi.org/10.3390/ijerph18126310>.
90. Kiro, V.V.; Gupta, A.; Singh, P.; Sharad, N.; Khurana, S.; Prakash, S.; Dar, L.; Malhotra, R.; Wig, N.; Kumar, A.; et al. Evaluation of COVID-19 Antigen Fluorescence Immunoassay Test for Rapid Detection of SARS-CoV-2. *J. Glob. Infect. Dis.* **2021**, *13*, 91–93. https://doi.org/10.4103/jgid.jgid_316_20.
91. Smith, R.L.; Gibson, L.L.; Martinez, P.P.; Ke, R.; Mirza, A.; Conte, M.; Gallagher, N.; Conte, A.; Wang, L.; Fredrickson, R.; et al. Longitudinal Assessment of Diagnostic Test Performance Over the Course of Acute SARS-CoV-2 Infection. *J. Infect. Dis.* **2021**, *224*, 976–982. <https://doi.org/10.1093/infdis/jiab337>.
92. L'Huillier, A.G.; Lacour, M.; Sadiku, D.; Gadiri, M.A.; De Siebenthal, L.; Schibler, M.; Eckerle, I.; Pinösch, S.; Kaiser, L.; Gervaix, A.; et al. Diagnostic Accuracy of SARS-CoV-2 Rapid Antigen Detection Testing in Symptomatic and Asymptomatic Children in the Clinical Setting. *J. Clin. Microbiol.* **2021**, *59*, e0099121. <https://doi.org/10.1128/jcm.00991-21>.
93. Gupta, A.; Anand, A.; Jain, N.; Goswami, S.; Anantharaj, A.; Patil, S.; Singh, R.; Kumar, A.; Shrivastava, T.; Bhatnagar, S.; et al. A novel G-quadruplex aptamer-based spike trimeric antigen test for the detection of SARS-CoV-2. *Mol. Nucleic Acids* **2021**, *26*, 321–332. <https://doi.org/10.1016/j.omtn.2021.06.014>.
94. Wagenhäuser, I.; Knies, K.; Rauschenberger, V.; Eisenmann, M.; McDonogh, M.; Petri, N.; Andres, O.; Flemming, S.; Gawlik, M.; Papsdorf, M.; et al. Clinical performance evaluation of SARS-CoV-2 rapid antigen testing in point of care usage in comparison to RT-qPCR. *EBioMedicine* **2021**, *69*, 103455. <https://doi.org/10.1016/j.ebiom.2021.103455>.
95. Fernández, M.D.; Estévez, A.S.; Alfonsín, F.L.; Arevalo, G.B. Usefulness of the Lumiradx™ Sars-Cov-2 antigen test in nursing home. *Enferm. Infecc. Microbiol. Clin.* **2021**. <https://doi.org/10.1016/j.eimc.2021.06.006>.
96. Amer, R.M.; Samir, M.; Gaber, O.A.; El-Deeb, N.A.; Abdelmoaty, A.A.; Ahmed, A.A.; Samy, W.; Atta, A.H.; Walaa, M.; Anis, R.H. Diagnostic performance of rapid antigen test for COVID-19 and the effect of viral load, sampling time, subject's clinical and laboratory parameters on test accuracy. *J. Infect. Public Health* **2021**, *14*, 1446–1453. <https://doi.org/10.1016/j.jiph.2021.06.002>.
97. Baccani, I.; Morecchiato, F.; Chilleri, C.; Cervini, C.; Gori, E.; Matarrese, D.; Bassetti, A.; Bonizzoli, M.; Mencarini, J.; Antonelli, A.; et al. Evaluation of Three Immunoassays for the Rapid Detection of SARS-CoV-2 antigens. *Diagn. Microbiol. Infect. Dis.* **2021**, *101*, 115434. <https://doi.org/10.1016/j.diagmicrobio.2021.115434>.

98. Matsuzaki, N.; Orihara, Y.; Kodana, M.; Kitagawa, Y.; Matsuoka, M.; Kawamura, R.; Takeuchi, S.; Imai, K.; Tarumoto, N.; Maesaki, S.; et al. Evaluation of a chemiluminescent enzyme immunoassay-based high-throughput SARS-CoV-2 antigen assay for the diagnosis of COVID-19: The VITROS® SARS-CoV-2 Antigen Test. *J. Med. Virol.* **2021**, *93*, 6778–6781. <https://doi.org/10.1002/jmv.27153>.
99. Jakobsen, K.K.; Jensen, J.S.; Todsén, T.; Tolsgaard, M.G.; Kirkby, N.; Lippert, F.; Vangsted, A.M.; Martel, C.J.; Klokke, M.; von Buchwald, C. Accuracy and cost description of rapid antigen test compared with reverse transcriptase-polymerase chain reaction for SARS-CoV-2 detection. *Dan. Med. J.* **2021**, *68*, A03210217.
100. Ngo Nsoga, M.T.; Kronig, I.; Perez Rodriguez, F.J.; Sattonnet-Roche, P.; Da Silva, D.; Helbling, J.; Sacks, J.A.; de Vos, M.; Boehm, E.; Gayet-Ageron, A.; et al. Diagnostic accuracy of Panbio rapid antigen tests on oropharyngeal swabs for detection of SARS-CoV-2. *PLoS ONE* **2021**, *16*, e0253321. <https://doi.org/10.1371/journal.pone.0253321>.
101. Smith, R.D.; Johnson, J.K.; Clay, C.; Girio-Herrera, L.; Stevens, D.; Abraham, M.; Zimand, P.; Ahlman, M.; Gimigliano, S.; Zhao, R.; et al. Clinical evaluation of Sofia Rapid Antigen Assay for detection of severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) among emergency department to hospital admissions. *Infect. Control Hosp. Epidemiol.* **2021**, 1–6. <https://doi.org/10.1017/ice.2021.281>.
102. Eleftheriou, I.; Dasoula, F.; Dimopoulou, D.; Lebessi, E.; Serafi, E.; Spyridis, N.; Tsolia, M. Real-life evaluation of a COVID-19 rapid antigen detection test in hospitalized children. *J. Med. Virol.* **2021**, *93*, 6040–6044. <https://doi.org/10.1002/jmv.27149>.
103. Lindner, A.K.; Nikolai, O.; Rohardt, C.; Kausch, F.; Wintel, M.; Gertler, M.; Burock, S.; Hörig, M.; Bernhard, J.; Tobian, F.; et al. Diagnostic accuracy and feasibility of patient self-testing with a SARS-CoV-2 antigen-detecting rapid test. *J. Clin. Virol.* **2021**, *141*, 104874. <https://doi.org/10.1016/j.jcv.2021.104874>.
104. Ferté, T.; Ramel, V.; Cazanave, C.; Lafon, M.E.; Bébéar, C.; Malvy, D.; Georges-Walryck, A.; Dehail, P. Accuracy of COVID-19 rapid antigenic tests compared to RT-PCR in a student population: The StudyCov study. *J. Clin. Virol.* **2021**, *141*, 104878. <https://doi.org/10.1016/j.jcv.2021.104878>.
105. Fernandez-Montero, A.; Argemi, J.; Rodríguez, J.A.; Ariño, A.H.; Moreno-Galarraga, L. Validation of a rapid antigen test as a screening tool for SARS-CoV-2 infection in asymptomatic populations. Sensitivity, specificity and predictive values. *EClinicalMedicine* **2021**, *37*, 100954. <https://doi.org/10.1016/j.eclinm.2021.100954>.
106. Hoehl, S.; Schenk, B.; Rudych, O.; Göttig, S.; Foppa, I.; Kohmer, N.; Karaca, O.; Toptan, T.; Ciesek, S. High-Frequency Self-Testing by Schoolteachers for Sars-Cov-2 Using a Rapid Antigen Test—Results of the Safe School Hesse study. *Dtsch. Arztebl. Int.* **2021**, *118*, 252–253. <https://doi.org/10.3238/arztebl.m2021.0187>.
107. Lee, J.; Kim, S.Y.; Huh, H.J.; Kim, N.; Sung, H.; Lee, H.; Roh, K.H.; Kim, T.S.; Hong, K.H. Clinical Performance of the Standard Q COVID-19 Rapid Antigen Test and Simulation of its Real-World Application in Korea. *Ann. Lab. Med.* **2021**, *41*, 588–592. <https://doi.org/10.3343/alm.2021.41.6.588>.
108. Mayanskiy, N.; Brzhozovskaya, E.; Fedorova, N.; Lebedin, Y. Parallel detection of SARS-CoV-2 RNA and nucleocapsid antigen in nasopharyngeal specimens from a COVID-19 patient screening cohort. *Int. J. Infect. Dis.* **2021**, *108*, 330–332. <https://doi.org/10.1016/j.ijid.2021.05.082>.
109. Leixner, G.; Voill-Glaninger, A.; Bonner, E.; Kreil, A.; Zadnikar, R.; Viveiros, A. Evaluation of the AMP SARS-CoV-2 rapid antigen test in a hospital setting. *Int. J. Infect. Dis.* **2021**, *108*, 353–356. <https://doi.org/10.1016/j.ijid.2021.05.063>.
110. Hirotsu, Y.; Sugiura, H.; Maejima, M.; Hayakawa, M.; Mochizuki, H.; Tsutsui, T.; Kakizaki, Y.; Miyashita, Y.; Omata, M. Comparison of Roche and Lumipulse quantitative SARS-CoV-2 antigen test performance using automated systems for the diagnosis of COVID-19. *Int. J. Infect. Dis.* **2021**, *108*, 263–269. <https://doi.org/10.1016/j.ijid.2021.05.067>.
111. Fiedler, M.; Holtkamp, C.; Dittmer, U.; Anastasiou, O.E. Performance of the LIAISON® SARS-CoV-2 Antigen Assay vs. SARS-CoV-2-RT-PCR. *Pathogens* **2021**, *10*, 658. <https://doi.org/10.3390/pathogens10060658>.
112. Dierks, S.; Bader, O.; Schwanbeck, J.; Groß, U.; Weig, M.S.; Mese, K.; Lugert, R.; Bohne, W.; Hahn, A.; Feltgen, N.; et al. Diagnosing SARS-CoV-2 with Antigen Testing, Transcription-Mediated Amplification and Real-Time PCR. *J. Clin. Med.* **2021**, *10*, 2404. <https://doi.org/10.3390/jcm10112404>.
113. Terpos, E.; Ntanasis-Stathopoulos, I.; Skvarč, M. Clinical Application of a New SARS-CoV-2 Antigen Detection Kit (Colloidal Gold) in the Detection of COVID-19. *Diagnostics* **2021**, *11*, 995. <https://doi.org/10.3390/diagnostics11060995>.
114. Osmanodja, B.; Budde, K.; Zickler, D.; Naik, M.G.; Hofmann, J.; Gertler, M.; Hülso, C.; Rössig, H.; Horn, P.; Seybold, J.; et al. Accuracy of a Novel SARS-CoV-2 Antigen-Detecting Rapid Diagnostic Test from Standardized Self-Collected Anterior Nasal Swabs. *J. Clin. Med.* **2021**, *10*, 2099. <https://doi.org/10.3390/jcm10102099>.
115. Harris, D.T.; Badowski, M.; Jernigan, B.; Sprissler, R.; Edwards, T.; Cohen, R.; Paul, S.; Merchant, N.; Weinkauf, C.C.; Bime, C.; et al. SARS-CoV-2 Rapid Antigen Testing of Symptomatic and Asymptomatic Individuals on the University of Arizona Campus. *Biomedicine* **2021**, *9*, 539. <https://doi.org/10.3390/biomedicine9050539>.
116. Cento, V.; Renica, S.; Matarazzo, E.; Antonello, M.; Colagrossi, L.; Di Ruscio, F.; Pani, A.; Fanti, D.; Vismara, C.; Puoti, M.; et al. Frontline Screening for SARS-CoV-2 Infection at Emergency Department Admission by Third Generation Rapid Antigen Test: Can We Spare RT-qPCR? *Viruses* **2021**, *13*, 818. <https://doi.org/10.3390/v13050818>.
117. Kumar, A.; Kunjukutty, R.; Thaha, A.; Srikumar, S.; Madhusoodanan, H.; David, S.; Biswas, L.; Sathyapalan, D. Universal screening for SARS-CoV-2 in pregnant women using a combination of antigen and RT-PCR testing. *Infez. Med.* **2021**, *29*, 294–296.
118. Orsi, A.; Pennati, B.M.; Bruzzzone, B.; Ricucci, V.; Ferone, D.; Barbera, P.; Arboscello, E.; Dentone, C.; Icardi, G. On-field evaluation of a ultra-rapid fluorescence immunoassay as a frontline test for SARS-CoV-2 diagnostic. *J. Virol. Methods* **2021**, *295*, 114201. <https://doi.org/10.1016/j.jviromet.2021.114201>.

119. Blairon, L.; Cupaiolo, R.; Thomas, I.; Piteüs, S.; Wilmet, A.; Beukinga, I.; Tré-Hardy, M. Efficacy comparison of three rapid antigen tests for SARS-CoV-2 and how viral load impact their performance. *J. Med. Virol.* **2021**, *93*, 5783–5788. <https://doi.org/10.1002/jmv.27108>.
120. Bornemann, L.; Kaup, O.; Kleideiter, J.; Panning, M.; Ruprecht, B.; Wehmeier, M. Real-life evaluation of the Sofia SARS-CoV-2 antigen assay in a large tertiary care hospital. *J. Clin. Virol.* **2021**, *140*, 104854. <https://doi.org/10.1016/j.jcv.2021.104854>.
121. Krüger, L.J.; Gaeddert, M.; Tobian, F.; Lainati, F.; Gottschalk, C.; Klein, J.A.F.; Schnitzler, P.; Kräusslich, H.G.; Nikolai, O.; Lindner, A.K.; et al. The Abbott PanBio WHO emergency use listed, rapid, antigen-detecting point-of-care diagnostic test for SARS-CoV-2-Evaluation of the accuracy and ease-of-use. *PLoS ONE* **2021**, *16*, e0247918. <https://doi.org/10.1371/journal.pone.0247918>.
122. Shaikh, N.; Friedlander, E.J.; Tate, P.J.; Liu, H.; Chang, C.H.; Wells, A.; Hoberman, A. Performance of a Rapid SARS-CoV-2 Antigen Detection Assay in Symptomatic Children. *Pediatrics* **2021**, *148*. <https://doi.org/10.1542/peds.2021-050832>.
123. Diez Flecha, C.; Rivero Rodríguez, A.M.; Fernández-Villa, T.; Fernández García, P.; Ferreira de Jesús, J.L.; Sánchez Antolín, G. Internal validity of a rapid test for COVID-19 antigens in a nursing home. *Semergen* **2021**, *47*, 332–336. <https://doi.org/10.1016/j.semerg.2021.04.003>.
124. Yokota, I.; Shane, P.Y.; Okada, K.; Unoki, Y.; Yang, Y.; Iwasaki, S.; Fujisawa, S.; Nishida, M.; Teshima, T. A novel strategy for SARS-CoV-2 mass screening with quantitative antigen testing of saliva: A diagnostic accuracy study. *Lancet Microbe* **2021**, *2*, e397–e404. [https://doi.org/10.1016/s2666-5247\(21\)00092-6](https://doi.org/10.1016/s2666-5247(21)00092-6).
125. Klein, J.A.F.; Krüger, L.J.; Tobian, F.; Gaeddert, M.; Lainati, F.; Schnitzler, P.; Lindner, A.K.; Nikolai, O.; Knorr, B.; Welker, A.; et al. Head-to-head performance comparison of self-collected nasal versus professional-collected nasopharyngeal swab for a WHO-listed SARS-CoV-2 antigen-detecting rapid diagnostic test. *Med. Microbiol. Immunol.* **2021**, *210*, 181–186. <https://doi.org/10.1007/s00430-021-00710-9>.
126. Caramello, V.; Boccuzzi, A.; Basile, V.; Ferraro, A.; Macciotta, A.; Catalano, A.; Costa, G.; Vineis, P.; Sacerdote, C.; Ricceri, F. Are antigenic tests useful for detecting SARS-CoV-2 infections in patients accessing to emergency departments? Results from a North-West Italy hospital. *J. Infect.* **2021**, *83*, 237–279. <https://doi.org/10.1016/j.jinf.2021.05.012>.
127. Koeleman, J.G.M.; Brand, H.; de Man, S.J.; Ong, D.S.Y. Clinical evaluation of rapid point-of-care antigen tests for diagnosis of SARS-CoV-2 infection. *Eur. J. Clin. Microbiol. Infect. Dis.* **2021**, *40*, 1975–1981. <https://doi.org/10.1007/s10096-021-04274-7>.
128. Šterbenc, A.; Tomič, V.; Bidovec Stojković, U.; Vrankar, K.; Rozman, A.; Zidarn, M. Usefulness of rapid antigen testing for SARS-CoV-2 screening of healthcare workers: A pilot study. *Clin. Exp. Med.* **2022**, *22*, 157–160. <https://doi.org/10.1007/s10238-021-00722-y>.
129. Kumar, K.K.; Sampritha, U.C.; Maganty, V.; Prakash, A.A.; Basumatary, J.; Adappa, K.; Chandraprabha, S.; Neeraja, T.G.; Guru Prasad, N.S.; Preethi, B.; et al. Pre-Operative SARS CoV-2 Rapid Antigen Test and Reverse Transcription Polymerase Chain Reaction: A conundrum in surgical decision making. *Indian J. Ophthalmol.* **2021**, *69*, 1560–1562. https://doi.org/10.4103/ijo.IJO_430_21.
130. Soleimani, R.; Deckers, C.; Huang, T.D.; Bogaerts, P.; Evrard, S.; Wallemme, I.; Habib, B.; Rouzé, P.; Denis, O. Rapid COVID-19 antigenic tests: Usefulness of a modified method for diagnosis. *J. Med. Virol.* **2021**, *93*, 5655–5659. <https://doi.org/10.1002/jmv.27094>.
131. Takeuchi, Y.; Akashi, Y.; Kato, D.; Kuwahara, M.; Muramatsu, S.; Ueda, A.; Notake, S.; Nakamura, K.; Ishikawa, H.; Suzuki, H. Diagnostic performance and characteristics of anterior nasal collection for the SARS-CoV-2 antigen test: A prospective study. *Sci. Rep.* **2021**, *11*, 10519. <https://doi.org/10.1038/s41598-021-90026-8>.
132. Homza, M.; Zelena, H.; Janosek, J.; Tomaskova, H.; Jezo, E.; Kloudova, A.; Mrazek, J.; Svagera, Z.; Prymula, R. Covid-19 antigen testing: Better than we know? A test accuracy study. *Infect. Dis.* **2021**, *53*, 661–668. <https://doi.org/10.1080/23744235.2021.1914857>.
133. Van der Moeren, N.; Zwart, V.F.; Lodder, E.B.; Van den Bijllaardt, W.; Van Esch, H.; Stohr, J.; Pot, J.; Welschen, I.; Van Mechelen, P.M.F.; Pas, S.D.; et al. Evaluation of the test accuracy of a SARS-CoV-2 rapid antigen test in symptomatic community dwelling individuals in the Netherlands. *PLoS ONE* **2021**, *16*, e0250886. <https://doi.org/10.1371/journal.pone.0250886>.
134. Brihn, A.; Chang, J.; Yong, K.O.; Balter, S.; Terashita, D.; Rubin, Z.; Yeganeh, N. Diagnostic Performance of an Antigen Test with RT-PCR for the Detection of SARS-CoV-2 in a Hospital Setting—Los Angeles County, California, June–August 2020. *MMWR Morb. Mortal. Wkly. Rep.* **2021**, *70*, 702–706. <https://doi.org/10.15585/mmwr.mm7019a3>.
135. Nordgren, J.; Sharma, S.; Olsson, H.; Jämtberg, M.; Falkeborn, T.; Svensson, L.; Hagbom, M. SARS-CoV-2 rapid antigen test: High sensitivity to detect infectious virus. *J. Clin. Virol.* **2021**, *140*, 104846. <https://doi.org/10.1016/j.jcv.2021.104846>.
136. Holzner, C.; Pabst, D.; Anastasiou, O.E.; Dittmer, U.; Manegold, R.K.; Risse, J.; Fistera, D.; Kill, C.; Falk, M. SARS-CoV-2 rapid antigen test: Fast-safe or dangerous? An analysis in the emergency department of an university hospital. *J. Med. Virol.* **2021**, *93*, 5323–5327. <https://doi.org/10.1002/jmv.27033>.
137. Kim, D.; Lee, J.; Bal, J.; Seo, S.K.; Chong, C.K.; Lee, J.H.; Park, H. Development and Clinical Evaluation of an Immunochromatography-Based Rapid Antigen Test (GenBody™ COVAG025) for COVID-19 Diagnosis. *Viruses* **2021**, *13*, 796. <https://doi.org/10.3390/v13050796>.
138. Bianco, G.; Boattini, M.; Barbui, A.M.; Scozzari, G.; Riccardini, F.; Coggiola, M.; Lupia, E.; Cavallo, R.; Costa, C. Evaluation of an antigen-based test for hospital point-of-care diagnosis of SARS-CoV-2 infection. *J. Clin. Virol.* **2021**, *139*, 104838. <https://doi.org/10.1016/j.jcv.2021.104838>.
139. Peña, M.; Ampuero, M.; Garcés, C.; Gaggero, A.; García, P.; Velasquez, M.S.; Luza, R.; Alvarez, P.; Paredes, F.; Acevedo, J.; et al. Performance of SARS-CoV-2 rapid antigen test compared with real-time RT-PCR in asymptomatic individuals. *Int. J. Infect. Dis.* **2021**, *107*, 201–204. <https://doi.org/10.1016/j.ijid.2021.04.087>.

140. Muhi, S.; Tayler, N.; Hoang, T.; Ballard, S.A.; Graham, M.; Rojek, A.; Kwong, J.C.; Trubiano, J.A.; Smibert, O.; Drewett, G.; et al. Multi-site assessment of rapid, point-of-care antigen testing for the diagnosis of SARS-CoV-2 infection in a low-prevalence setting: A validation and implementation study. *Lancet Reg. Health West Pac.* **2021**, *9*, 100115. <https://doi.org/10.1016/j.lanwpc.2021.100115>.
141. Uwamino, Y.; Nagata, M.; Aoki, W.; Nakagawa, T.; Inose, R.; Yokota, H.; Furusawa, Y.; Sakai-Tagawa, Y.; Iwatsuki-Horimoto, K.; Kawaoka, Y.; et al. Accuracy of rapid antigen detection test for nasopharyngeal swab specimens and saliva samples in comparison with RT-PCR and viral culture for SARS-CoV-2 detection. *J. Infect. Chemother.* **2021**, *27*, 1058–1062. <https://doi.org/10.1016/j.jiac.2021.04.010>.
142. Thakur, P.; Saxena, S.; Manchanda, V.; Rana, N.; Goel, R.; Arora, R. Utility of Antigen-Based Rapid Diagnostic Test for Detection of SARS-CoV-2 Virus in Routine Hospital Settings. *Lab. Med.* **2021**, *52*, e154–e158. <https://doi.org/10.1093/labmed/lmab033>.
143. Homza, M.; Zelena, H.; Janosek, J.; Tomaskova, H.; Jezo, E.; Kloudova, A.; Mrazek, J.; Svagera, Z.; Prymula, R. Five Antigen Tests for SARS-CoV-2: Virus Viability Matters. *Viruses* **2021**, *13*, 684. <https://doi.org/10.3390/v13040684>.
144. Shah, M.M.; Salvatore, P.P.; Ford, L.; Kamitani, E.; Whaley, M.J.; Mitchell, K.; Currie, D.W.; Morgan, C.N.; Segaloff, H.E.; Lecher, S.; et al. Performance of Repeat BinaxNOW Severe Acute Respiratory Syndrome Coronavirus 2 Antigen Testing in a Community Setting, Wisconsin, November 2020–December 2020. *Clin. Infect. Dis.* **2021**, *73*, S54–S57. <https://doi.org/10.1093/cid/ciab309>.
145. McKay, S.L.; Tobolowsky, F.A.; Moritz, E.D.; Hatfield, K.M.; Bhatnagar, A.; LaVoie, S.P.; Jackson, D.A.; Lecy, K.D.; Bryant-Genevier, J.; Campbell, D.; et al. Performance Evaluation of Serial SARS-CoV-2 Rapid Antigen Testing During a Nursing Home Outbreak. *Ann. Intern. Med.* **2021**, *174*, 945–951. <https://doi.org/10.7326/m21-0422>.
146. Yin, N.; Debuysschere, C.; Decroly, M.; Bouazza, F.Z.; Collot, V.; Martin, C.; Ponthieux, F.; Dahma, H.; Gilbert, M.; Wautier, M.; et al. SARS-CoV-2 Diagnostic Tests: Algorithm and Field Evaluation From the Near Patient Testing to the Automated Diagnostic Platform. *Front. Med.* **2021**, *8*, 650581. <https://doi.org/10.3389/fmed.2021.650581>.
147. Baro, B.; Rodo, P.; Ouchi, D.; Bordoy, A.E.; Saya Amaro, E.N.; Salsench, S.V.; Molinos, S.; Alemany, A.; Ubals, M.; Corbacho-Monné, M.; et al. Performance characteristics of five antigen-detecting rapid diagnostic test (Ag-RDT) for SARS-CoV-2 asymptomatic infection: A head-to-head benchmark comparison. *J. Infect.* **2021**, *82*, 269–275. <https://doi.org/10.1016/j.jinf.2021.04.009>.
148. Caputo, V.; Bax, C.; Colantoni, L.; Peconi, C.; Termine, A.; Fabrizio, C.; Calvino, G.; Luzzi, L.; Panunzi, G.G.; Fusco, C.; et al. Comparative analysis of antigen and molecular tests for the detection of Sars-CoV-2 and related variants: A study on 4266 samples. *Int. J. Infect. Dis.* **2021**, *108*, 187–189. <https://doi.org/10.1016/j.ijid.2021.04.048>.
149. Kenyeres, B.; Ánosi, N.; Bányai, K.; Mátyus, M.; Orosz, L.; Kiss, A.; Kele, B.; Burián, K.; Lengyel, G. Comparison of four PCR and two point of care assays used in the laboratory detection of SARS-CoV-2. *J. Virol. Methods* **2021**, *293*, 114165. <https://doi.org/10.1016/j.jviromet.2021.114165>.
150. Häuser, F.; Sprinzl, M.F.; Dreis, K.J.; Renzaho, A.; Youhanen, S.; Kremer, W.M.; Podlech, J.; Galle, P.R.; Lackner, K.J.; Rossmann, H.; et al. Evaluation of a laboratory-based high-throughput SARS-CoV-2 antigen assay for non-COVID-19 patient screening at hospital admission. *Med. Microbiol. Immunol.* **2021**, *210*, 165–171. <https://doi.org/10.1007/s00430-021-00706-5>.
151. Lefever, S.; Indevuyst, C.; Cuyppers, L.; Dewaele, K.; Yin, N.; Cotton, F.; Padalko, E.; Oyaert, M.; Descy, J.; Cavalier, E.; et al. Comparison of the Quantitative DiaSorin Liaison Antigen Test to Reverse Transcription-PCR for the Diagnosis of COVID-19 in Symptomatic and Asymptomatic Outpatients. *J. Clin. Microbiol.* **2021**, *59*, e0037421. <https://doi.org/10.1128/jcm.00374-21>.
152. Zacharias, M.; Stangl, V.; Thüringer, A.; Loibner, M.; Wurm, P.; Wolfgruber, S.; Zatloukal, K.; Kashofer, K.; Gorkiewicz, G. Rapid Antigen Test for Postmortem Evaluation of SARS-CoV-2 Carriage. *Emerg. Infect. Dis.* **2021**, *27*, 1734–1737. <https://doi.org/10.3201/eid2706.210226>.
153. Oh, S.M.; Jeong, H.; Chang, E.; Choe, P.G.; Kang, C.K.; Park, W.B.; Kim, T.S.; Kwon, W.Y.; Oh, M.D.; Kim, N.J. Clinical Application of the Standard Q COVID-19 Ag Test for the Detection of SARS-CoV-2 Infection. *J. Korean Med. Sci.* **2021**, *36*, e101. <https://doi.org/10.3346/jkms.2021.36.e101>.
154. Asai, N.; Sakanashi, D.; Ohashi, W.; Nakamura, A.; Kawamoto, Y.; Miyazaki, N.; Ohno, T.; Yamada, A.; Chida, S.; Shibata, Y.; et al. Efficacy and validity of automated quantitative chemiluminescent enzyme immunoassay for SARS-CoV-2 antigen test from saliva specimen in the diagnosis of COVID-19. *J. Infect. Chemother.* **2021**, *27*, 1039–1042. <https://doi.org/10.1016/j.jiac.2021.03.021>.
155. Kweon, O.J.; Lim, Y.K.; Kim, H.R.; Choi, Y.; Kim, M.C.; Choi, S.H.; Chung, J.W.; Lee, M.K. Evaluation of rapid SARS-CoV-2 antigen tests, AFIAS COVID-19 Ag and ichroma COVID-19 Ag, with serial nasopharyngeal specimens from COVID-19 patients. *PLoS ONE* **2021**, *16*, e0249972. <https://doi.org/10.1371/journal.pone.0249972>.
156. Menchinelli, G.; Bordi, L.; Liotti, F.M.; Palucci, I.; Capobianchi, M.R.; Sberna, G.; Lalle, E.; Romano, L.; De Angelis, G.; Marchetti, S.; et al. Lumipulse G SARS-CoV-2 Ag assay evaluation using clinical samples from different testing groups. *Clin. Chem. Lab. Med.* **2021**, *59*, 1468–1476. <https://doi.org/10.1515/cclm-2021-0182>.
157. Sood, N.; Shetgiri, R.; Rodriguez, A.; Jimenez, D.; Treminino, S.; Daflos, A.; Simon, P. Evaluation of the Abbott BinaxNOW rapid antigen test for SARS-CoV-2 infection in children: Implications for screening in a school setting. *PLoS ONE* **2021**, *16*, e0249710. <https://doi.org/10.1371/journal.pone.0249710>.
158. Epstude, J.; Skiba, M.; Harsch, I.A. Antibody titers and rapid antigen testing in elderly patients with SARS-CoV-2 pneumonia vs. staff of ICU and “Covid-19” wards. *GMS Hyg. Infect. Control* **2021**, *16*, Doc11. <https://doi.org/10.3205/dgkh000382>.
159. Berger, A.; Nsoga, M.T.N.; Perez-Rodriguez, F.J.; Aad, Y.A.; Sattonnet-Roche, P.; Gayet-Ageron, A.; Jaksic, C.; Torriani, G.; Boehm, E.; Kronig, I.; et al. Diagnostic accuracy of two commercial SARS-CoV-2 antigen-detecting rapid tests at the point of care in community-based testing centers. *PLoS ONE* **2021**, *16*, e0248921. <https://doi.org/10.1371/journal.pone.0248921>.

160. Matsuda, E.M.; de Campos, I.B.; de Oliveira, I.P.; Colpas, D.R.; Carmo, A.; Brígido, L.F.M. Field evaluation of COVID-19 antigen tests versus RNA based detection: Potential lower sensitivity compensated by immediate results, technical simplicity, and low cost. *J. Med. Virol.* **2021**, *93*, 4405–4410. <https://doi.org/10.1002/jmv.26985>.
161. Van Honacker, E.; Van Vaerenbergh, K.; Boel, A.; De Beenhouwer, H.; Leroux-Roels, I.; Cattoir, L. Comparison of five SARS-CoV-2 rapid antigen detection tests in a hospital setting and performance of one antigen assay in routine practice: A useful tool to guide isolation precautions? *J. Hosp. Infect.* **2021**, *114*, 144–152. <https://doi.org/10.1016/j.jhin.2021.03.021>.
162. Boum, Y.; Fai, K.N.; Nikolay, B.; Mboringong, A.B.; Bebell, L.M.; Ndifon, M.; Abbah, A.; Essaka, R.; Eteki, L.; Luquero, F.; et al. Performance and operational feasibility of antigen and antibody rapid diagnostic tests for COVID-19 in symptomatic and asymptomatic patients in Cameroon: A clinical, prospective, diagnostic accuracy study. *Lancet Infect. Dis.* **2021**, *21*, 1089–1096. [https://doi.org/10.1016/s1473-3099\(21\)00132-8](https://doi.org/10.1016/s1473-3099(21)00132-8).
163. Mboumba Bouassa, R.S.; Veyer, D.; Péré, H.; Bélec, L. Analytical performances of the point-of-care SIENNA™ COVID-19 Antigen Rapid Test for the detection of SARS-CoV-2 nucleocapsid protein in nasopharyngeal swabs: A prospective evaluation during the COVID-19 second wave in France. *Int. J. Infect. Dis.* **2021**, *106*, 8–12. <https://doi.org/10.1016/j.ijid.2021.03.051>.
164. Stokes, W.; Berenger, B.M.; Portnoy, D.; Scott, B.; Szelewicki, J.; Singh, T.; Venner, A.A.; Turnbull, L.; Pabbaraju, K.; Shokoples, S.; et al. Clinical performance of the Abbott Panbio with nasopharyngeal, throat, and saliva swabs among symptomatic individuals with COVID-19. *Eur. J. Clin. Microbiol. Infect. Dis.* **2021**, *40*, 1721–1726. <https://doi.org/10.1007/s10096-021-04202-9>.
165. Landaas, E.T.; Storm, M.L.; Tollånes, M.C.; Barlinn, R.; Kran, A.B.; Bragstad, K.; Christensen, A.; Andreassen, T. Diagnostic performance of a SARS-CoV-2 rapid antigen test in a large, Norwegian cohort. *J. Clin. Virol.* **2021**, *137*, 104789. <https://doi.org/10.1016/j.jcv.2021.104789>.
166. Takeuchi, Y.; Akashi, Y.; Kato, D.; Kuwahara, M.; Muramatsu, S.; Ueda, A.; Notake, S.; Nakamura, K.; Ishikawa, H.; Suzuki, H. The evaluation of a newly developed antigen test (QuickNavi™-COVID19 Ag) for SARS-CoV-2: A prospective observational study in Japan. *J. Infect. Chemother.* **2021**, *27*, 890–894. <https://doi.org/10.1016/j.jiac.2021.02.029>.
167. Igloi, Z.; Velzing, J.; van Beek, J.; van de Vijver, D.; Aron, G.; Ensing, R.; Benschop, K.; Han, W.; Boelsums, T.; Koopmans, M.; et al. Clinical Evaluation of Roche SD Biosensor Rapid Antigen Test for SARS-CoV-2 in Municipal Health Service Testing Site, the Netherlands. *Emerg. Infect. Dis.* **2021**, *27*, 1323–1329. <https://doi.org/10.3201/eid2705.204688>.
168. Masiá, M.; Fernández-González, M.; Sánchez, M.; Carvajal, M.; García, J.A.; Gonzalo-Jiménez, N.; Ortiz de la Tabla, V.; Agulló, V.; Candela, I.; Guijarro, J.; et al. Nasopharyngeal Panbio COVID-19 Antigen Performed at Point-of-Care Has a High Sensitivity in Symptomatic and Asymptomatic Patients With Higher Risk for Transmission and Older Age. *Open Forum Infect. Dis.* **2021**, *8*, ofab059. <https://doi.org/10.1093/ofid/ofab059>.
169. Jääskeläinen, A.E.; Ahava, M.J.; Jokela, P.; Szivovics, L.; Pohjala, S.; Vapalahti, O.; Lappalainen, M.; Hepojoki, J.; Kurkela, S. Evaluation of three rapid lateral flow antigen detection tests for the diagnosis of SARS-CoV-2 infection. *J. Clin. Virol.* **2021**, *137*, 104785. <https://doi.org/10.1016/j.jcv.2021.104785>.
170. Olearo, F.; Nörz, D.; Heinrich, F.; Sutter, J.P.; Roedl, K.; Schultze, A.; Wiesch, J.S.Z.; Braun, P.; Oestereich, L.; Kreuels, B.; et al. Handling and accuracy of four rapid antigen tests for the diagnosis of SARS-CoV-2 compared to RT-qPCR. *J. Clin. Virol.* **2021**, *137*, 104782. <https://doi.org/10.1016/j.jcv.2021.104782>.
171. Ishii, T.; Sasaki, M.; Yamada, K.; Kato, D.; Osuka, H.; Aoki, K.; Morita, T.; Ishii, Y.; Tateda, K. Immunochromatography and chemiluminescent enzyme immunoassay for COVID-19 diagnosis. *J. Infect. Chemother.* **2021**, *27*, 915–918. <https://doi.org/10.1016/j.jiac.2021.02.025>.
172. Peña-Rodríguez, M.; Viera-Segura, O.; García-Chagollán, M.; Zepeda-Nuño, J.S.; Muñoz-Valle, J.F.; Mora-Mora, J.; Espinoza-De León, G.; Bustillo-Armendáriz, G.; García-Cedillo, F.; Vega-Magaña, N. Performance evaluation of a lateral flow assay for nasopharyngeal antigen detection for SARS-CoV-2 diagnosis. *J. Clin. Lab. Anal.* **2021**, *35*, e23745. <https://doi.org/10.1002/jcla.23745>.
173. Gili, A.; Paggi, R.; Russo, C.; Cenci, E.; Pietrella, D.; Graziani, A.; Stracci, F.; Mencacci, A. Evaluation of Lumipulse® G SARS-CoV-2 antigen assay automated test for detecting SARS-CoV-2 nucleocapsid protein (NP) in nasopharyngeal swabs for community and population screening. *Int. J. Infect. Dis.* **2021**, *105*, 391–396. <https://doi.org/10.1016/j.ijid.2021.02.098>.
174. Pérez-García, F.; Romanyk, J.; Gómez-Herruz, P.; Arroyo, T.; Pérez-Tanoira, R.; Linares, M.; Pérez Ranz, I.; Labrador Ballester, A.; Moya Gutiérrez, H.; Ruiz-Álvarez, M.J.; et al. Diagnostic performance of CerTest and Panbio antigen rapid diagnostic tests to diagnose SARS-CoV-2 infection. *J. Clin. Virol.* **2021**, *137*, 104781. <https://doi.org/10.1016/j.jcv.2021.104781>.
175. Kilic, A.; Hiestand, B.; Palavecino, E. Evaluation of Performance of the BD Veritor SARS-CoV-2 Chromatographic Immunoassay Test in Patients with Symptoms of COVID-19. *J. Clin. Microbiol.* **2021**, *59*, e00260-21. <https://doi.org/10.1128/jcm.00260-21>.
176. Drain, P.K.; Ampajwala, M.; Chappel, C.; Gvozden, A.B.; Hoppers, M.; Wang, M.; Rosen, R.; Young, S.; Zissman, E.; Montano, M. A Rapid, High-Sensitivity SARS-CoV-2 Nucleocapsid Immunoassay to Aid Diagnosis of Acute COVID-19 at the Point of Care: A Clinical Performance Study. *Infect. Dis. Ther.* **2021**, *10*, 753–761. <https://doi.org/10.1007/s40121-021-00413-x>.
177. Basso, D.; Aita, A.; Padoan, A.; Cosma, C.; Navaglia, F.; Moz, S.; Contran, N.; Zambon, C.F.; Maria Cattelan, A.; Plebani, M. Salivary SARS-CoV-2 antigen rapid detection: A prospective cohort study. *Clin. Chim. Acta* **2021**, *517*, 54–59. <https://doi.org/10.1016/j.cca.2021.02.014>.
178. Pollock, N.R.; Jacobs, J.R.; Tran, K.; Cranston, A.E.; Smith, S.; O’Kane, C.Y.; Roady, T.J.; Moran, A.; Scarry, A.; Carroll, M.; et al. Performance and Implementation Evaluation of the Abbott BinaxNOW Rapid Antigen Test in a High-Throughput Drive-Through Community Testing Site in Massachusetts. *J. Clin. Microbiol.* **2021**, *59*, e00083-21. <https://doi.org/10.1128/jcm.00083-21>.

179. Ristić, M.; Nikolić, N.; Čabarkapa, V.; Turkulov, V.; Petrović, V. Validation of the Standard Q COVID-19 antigen test in Vojvodina, Serbia. *PLoS ONE* **2021**, *16*, e0247606. <https://doi.org/10.1371/journal.pone.0247606>.
180. Courtellemont, L.; Guinard, J.; Guillaume, C.; Giaché, S.; Rzepecki, V.; Seve, A.; Gubavu, C.; Baud, K.; Le Helloco, C.; Cassuto, G.N.; et al. High performance of a novel antigen detection test on nasopharyngeal specimens for diagnosing SARS-CoV-2 infection. *J. Med. Virol.* **2021**, *93*, 3152–3157. <https://doi.org/10.1002/jmv.26896>.
181. Thommes, L.; Burkert, F.R.; Öttl, K.W.; Goldin, D.; Loacker, L.; Lanser, L.; Griesmacher, A.; Theurl, I.; Weiss, G.; Bellmann-Weiler, R. Comparative evaluation of four SARS-CoV-2 antigen tests in hospitalized patients. *Int. J. Infect. Dis.* **2021**, *105*, 144–146. <https://doi.org/10.1016/j.ijid.2021.02.052>.
182. González-Donapetry, P.; García-Clemente, P.; Bloise, I.; García-Sánchez, C.; Sánchez Castellano, M.; Romero, M.P.; Gutiérrez Arroyo, A.; Mingorance, J.; de Ceano-Vivas La Calle, M.; García-Rodríguez, J. Think of the Children: Evaluation of SARS-CoV-2 Rapid Antigen Test in Pediatric Population. *Pediatr. Infect. Dis. J.* **2021**, *40*, 385–388. <https://doi.org/10.1097/inf.0000000000003101>.
183. Eshghifar, N.; Busheri, A.; Shrestha, R.; Beqaj, S. Evaluation of Analytical Performance of Seven Rapid Antigen Detection Kits for Detection of SARS-CoV-2 Virus. *Int. J. Gen. Med.* **2021**, *14*, 435–440. <https://doi.org/10.2147/ijgm.S297762>.
184. Merino, P.; Guinea, J.; Muñoz-Gallego, I.; González-Donapetry, P.; Galán, J.C.; Antona, N.; Cilla, G.; Hernández-Crespo, S.; Díaz-de Tuesta, J.L.; Gual-de Torrella, A.; et al. Multicenter evaluation of the Panbio™ COVID-19 rapid antigen-detection test for the diagnosis of SARS-CoV-2 infection. *Clin. Microbiol. Infect.* **2021**, *27*, 758–761. <https://doi.org/10.1016/j.cmi.2021.02.001>.
185. Bulilete, O.; Lorente, P.; Leiva, A.; Carandell, E.; Oliver, A.; Rojo, E.; Pericas, P.; Llobera, J. Panbio™ rapid antigen test for SARS-CoV-2 has acceptable accuracy in symptomatic patients in primary health care. *J. Infect.* **2021**, *82*, 391–398. <https://doi.org/10.1016/j.jinf.2021.02.014>.
186. Torres, I.; Poujois, S.; Albert, E.; Álvarez, G.; Colomina, J.; Navarro, D. Point-of-care evaluation of a rapid antigen test (CLINITEST®) Rapid COVID-19 Antigen Test) for diagnosis of SARS-CoV-2 infection in symptomatic and asymptomatic individuals. *J. Infect.* **2021**, *82*, e11–e12. <https://doi.org/10.1016/j.jinf.2021.02.010>.
187. Lindner, A.K.; Nikolai, O.; Rohardt, C.; Burock, S.; Hülso, C.; Bölke, A.; Gertler, M.; Krüger, L.J.; Gaeddert, M.; Tobian, F.; et al. Head-to-head comparison of SARS-CoV-2 antigen-detecting rapid test with professional-collected nasal versus nasopharyngeal swab. *Eur. Respir. J.* **2021**, *57*. <https://doi.org/10.1183/13993003.04430-2020>.
188. Hirotsu, Y.; Maejima, M.; Shibusawa, M.; Amemiya, K.; Nagakubo, Y.; Hosaka, K.; Sueki, H.; Hayakawa, M.; Mochizuki, H.; Tsutsui, T.; et al. Prospective study of 1308 nasopharyngeal swabs from 1033 patients using the LUMIPULSE SARS-CoV-2 antigen test: Comparison with RT-qPCR. *Int. J. Infect. Dis.* **2021**, *105*, 7–14. <https://doi.org/10.1016/j.ijid.2021.02.005>.
189. Salvagno, G.L.; Gianfilippi, G.; Bragantini, D.; Henry, B.M.; Lippi, G. Clinical assessment of the Roche SARS-CoV-2 rapid antigen test. *Diagnosis* **2021**, *8*, 322–326. <https://doi.org/10.1515/dx-2020-0154>.
190. Veyrenche, N.; Bolloré, K.; Pisoni, A.; Bedin, A.S.; Mondain, A.M.; Ducos, J.; Segondy, M.; Montes, B.; Pastor, P.; Morquin, D.; et al. Diagnosis value of SARS-CoV-2 antigen/antibody combined testing using rapid diagnostic tests at hospital admission. *J. Med. Virol.* **2021**, *93*, 3069–3076. <https://doi.org/10.1002/jmv.26855>.
191. Porte, L.; Legarraga, P.; Iruretagoyena, M.; Vollrath, V.; Pizarro, G.; Munita, J.; Araos, R.; Weitzel, T. Evaluation of two fluorescence immunoassays for the rapid detection of SARS-CoV-2 antigen-new tool to detect infective COVID-19 patients. *PeerJ* **2021**, *9*, e10801. <https://doi.org/10.7717/peerj.10801>.
192. Domínguez Fernández, M.; Peña Rodríguez, M.F.; Lamelo Alfonsín, F.; Bou Arévalo, G. Experience with Panbio™ rapid antigens test device for the detection of SARS-CoV-2 in nursing homes. *Enferm. Infecc. Microbiol. Clin.* **2021**, *40*, 42–43. <https://doi.org/10.1016/j.eimc.2020.12.008>.
193. Kobayashi, R.; Murai, R.; Asanuma, K.; Fujiya, Y.; Takahashi, S. Evaluating a novel, highly sensitive, and quantitative reagent for detecting SARS-CoV-2 antigen. *J. Infect. Chemother.* **2021**, *27*, 800–807. <https://doi.org/10.1016/j.jiac.2021.01.007>.
194. Houston, H.; Gupta-Wright, A.; Toke-Bjølgerud, E.; Biggin-Lamming, J.; John, L. Diagnostic accuracy and utility of SARS-CoV-2 antigen lateral flow assays in medical admissions with possible COVID-19. *J. Hosp. Infect.* **2021**, *110*, 203–205. <https://doi.org/10.1016/j.jhin.2021.01.018>.
195. Ciotti, M.; Maurici, M.; Pieri, M.; Andreoni, M.; Bernardini, S. Performance of a rapid antigen test in the diagnosis of SARS-CoV-2 infection. *J. Med. Virol.* **2021**, *93*, 2988–2991. <https://doi.org/10.1002/jmv.26830>.
196. Okoye, N.C.; Barker, A.P.; Curtis, K.; Orlandi, R.R.; Snavelly, E.A.; Wright, C.; Hanson, K.E.; Pearson, L.N. Performance Characteristics of BinaxNOW COVID-19 Antigen Card for Screening Asymptomatic Individuals in a University Setting. *J. Clin. Microbiol.* **2021**, *59*, e03282–20. <https://doi.org/10.1128/jcm.03282-20>.
197. James, A.E.; Gulley, T.; Kothari, A.; Holder, K.; Garner, K.; Patil, N. Performance of the BinaxNOW coronavirus disease 2019 (COVID-19) Antigen Card test relative to the severe acute respiratory coronavirus virus 2 (SARS-CoV-2) real-time reverse transcriptase polymerase chain reaction (rRT-PCR) assay among symptomatic and asymptomatic healthcare employees. *Infect. Control Hosp. Epidemiol.* **2022**, *43*, 99–101. <https://doi.org/10.1017/ice.2021.20>.
198. Villaverde, S.; Domínguez-Rodríguez, S.; Sabrido, G.; Pérez-Jorge, C.; Plata, M.; Romero, M.P.; Grasa, C.D.; Jiménez, A.B.; Heras, E.; Broncano, A.; et al. Diagnostic Accuracy of the Panbio Severe Acute Respiratory Syndrome Coronavirus 2 Antigen Rapid Test Compared with Reverse-Transcriptase Polymerase Chain Reaction Testing of Nasopharyngeal Samples in the Pediatric Population. *J. Pediatr.* **2021**, *232*, 287–289.e284. <https://doi.org/10.1016/j.jpeds.2021.01.027>.

199. Pekosz, A.; Parvu, V.; Li, M.; Andrews, J.C.; Manabe, Y.C.; Kodosi, S.; Gary, D.S.; Roger-Dalbert, C.; Leitch, J.; Cooper, C.K. Antigen-Based Testing but Not Real-Time Polymerase Chain Reaction Correlates with Severe Acute Respiratory Syndrome Coronavirus 2 Viral Culture. *Clin. Infect. Dis.* **2021**, *73*, e2861–e2866. <https://doi.org/10.1093/cid/ciaa1706>.
200. Kohmer, N.; Toptan, T.; Pallas, C.; Karaca, O.; Pfeiffer, A.; Westhaus, S.; Widera, M.; Berger, A.; Hoehl, S.; Kammel, M.; et al. The Comparative Clinical Performance of Four SARS-CoV-2 Rapid Antigen Tests and Their Correlation to Infectivity In Vitro. *J. Clin. Med.* **2021**, *10*, 328. <https://doi.org/10.3390/jcm10020328>.
201. Prince-Guerra, J.L.; Almendares, O.; Nolen, L.D.; Gunn, J.K.L.; Dale, A.P.; Buono, S.A.; Deutsch-Feldman, M.; Suppiah, S.; Hao, L.; Zeng, Y.; et al. Evaluation of Abbott BinaxNOW Rapid Antigen Test for SARS-CoV-2 Infection at Two Community-Based Testing Sites—Pima County, Arizona, 3–17 November 2020. *MMWR Morb. Mortal. Wkly. Rep.* **2021**, *70*, 100–105. <https://doi.org/10.15585/mmwr.mm7003e3>.
202. Möckel, M.; Corman, V.M.; Stegemann, M.S.; Hofmann, J.; Stein, A.; Jones, T.C.; Gastmeier, P.; Seybold, J.; Offermann, R.; Bachmann, U.; et al. SARS-CoV-2 antigen rapid immunoassay for diagnosis of COVID-19 in the emergency department. *Biomarkers* **2021**, *26*, 213–220. <https://doi.org/10.1080/1354750x.2021.1876769>.
203. Rottenstreich, A.; Zarbiv, G.; Kabiri, D.; Porat, S.; Sompolsky, Y.; Reubinoff, B.; Benenson, S.; Oster, Y. Rapid antigen detection testing for universal screening for severe acute respiratory syndrome coronavirus 2 in women admitted for delivery. *Am. J. Obstet. Gynecol.* **2021**, *224*, 539–540. <https://doi.org/10.1016/j.ajog.2021.01.002>.
204. Favresse, J.; Gillot, C.; Oliveira, M.; Cadrobbi, J.; Elsen, M.; Eucher, C.; Laffineur, K.; Rosseels, C.; Van Eeckhoudt, S.; Nicolas, J.B.; et al. Head-to-Head Comparison of Rapid and Automated Antigen Detection Tests for the Diagnosis of SARS-CoV-2 Infection. *J. Clin. Med.* **2021**, *10*, 265. <https://doi.org/10.3390/jcm10020265>.
205. Osterman, A.; Baldauf, H.M.; Eleteby, M.; Wettengel, J.M.; Afridi, S.Q.; Fuchs, T.; Holzmann, E.; Maier, A.; Döring, J.; Grzimek-Koschewa, N.; et al. Evaluation of two rapid antigen tests to detect SARS-CoV-2 in a hospital setting. *Med. Microbiol. Immunol.* **2021**, *210*, 65–72. <https://doi.org/10.1007/s00430-020-00698-8>.
206. Pollock, N.R.; Savage, T.J.; Wardell, H.; Lee, R.A.; Mathew, A.; Stengelin, M.; Sigal, G.B. Correlation of SARS-CoV-2 Nucleocapsid Antigen and RNA Concentrations in Nasopharyngeal Samples from Children and Adults Using an Ultrasensitive and Quantitative Antigen Assay. *J. Clin. Microbiol.* **2021**, *59*, e03077–20. <https://doi.org/10.1128/jcm.03077-20>.
207. Aoki, K.; Nagasawa, T.; Ishii, Y.; Yagi, S.; Okuma, S.; Kashiwagi, K.; Maeda, T.; Miyazaki, T.; Yoshizawa, S.; Tateda, K. Clinical validation of quantitative SARS-CoV-2 antigen assays to estimate SARS-CoV-2 viral loads in nasopharyngeal swabs. *J. Infect. Chemother.* **2021**, *27*, 613–616. <https://doi.org/10.1016/j.jiac.2020.11.021>.
208. Torres, I.; Poujois, S.; Albert, E.; Colomina, J.; Navarro, D. Evaluation of a rapid antigen test (Panbio™ COVID-19 Ag rapid test device) for SARS-CoV-2 detection in asymptomatic close contacts of COVID-19 patients. *Clin. Microbiol. Infect.* **2021**, *27*, 636.e631–636.e634. <https://doi.org/10.1016/j.cmi.2020.12.022>.
209. Alemany, A.; Baró, B.; Ouchi, D.; Rodó, P.; Ubals, M.; Corbacho-Monné, M.; Vergara-Alert, J.; Rodon, J.; Segalés, J.; Esteban, C.; et al. Analytical and clinical performance of the panbio COVID-19 antigen-detecting rapid diagnostic test. *J. Infect.* **2021**, *82*, 186–230. <https://doi.org/10.1016/j.jinf.2020.12.033>.
210. Rastawicki, W.; Gierczyński, R.; Juszczak, G.; Mitura, K.; Henry, B.M. Evaluation of PCL rapid point of care antigen test for detection of SARS-CoV-2 in nasopharyngeal swabs. *J. Med. Virol.* **2021**, *93*, 1920–1922. <https://doi.org/10.1002/jmv.26765>.
211. Yamamoto, K.; Suzuki, M.; Yamada, G.; Sudo, T.; Nomoto, H.; Kinoshita, N.; Nakamura, K.; Tsujimoto, Y.; Kusaba, Y.; Morita, C.; et al. Utility of the antigen test for coronavirus disease 2019: Factors influencing the prediction of the possibility of disease transmission. *Int. J. Infect. Dis.* **2021**, *104*, 65–72. <https://doi.org/10.1016/j.ijid.2020.12.079>.
212. Kashiwagi, K.; Ishii, Y.; Aoki, K.; Yagi, S.; Maeda, T.; Miyazaki, T.; Yoshizawa, S.; Aoyagi, K.; Tateda, K. Immunochromatographic test for the detection of SARS-CoV-2 in saliva. *J. Infect. Chemother.* **2021**, *27*, 384–386. <https://doi.org/10.1016/j.jiac.2020.11.016>.
213. Pilarowski, G.; Lebel, P.; Sunshine, S.; Liu, J.; Crawford, E.; Marquez, C.; Rubio, L.; Chamie, G.; Martinez, J.; Peng, J.; et al. Performance Characteristics of a Rapid Severe Acute Respiratory Syndrome Coronavirus 2 Antigen Detection Assay at a Public Plaza Testing Site in San Francisco. *J. Infect. Dis.* **2021**, *223*, 1139–1144. <https://doi.org/10.1093/infdis/jiaa802>.
214. Aoki, K.; Nagasawa, T.; Ishii, Y.; Yagi, S.; Kashiwagi, K.; Miyazaki, T.; Tateda, K. Evaluation of clinical utility of novel coronavirus antigen detection reagent, Espline® SARS-CoV-2. *J. Infect. Chemother.* **2021**, *27*, 319–322. <https://doi.org/10.1016/j.jiac.2020.11.015>.
215. Pray, I.W.; Ford, L.; Cole, D.; Lee, C.; Bigouette, J.P.; Abedi, G.R.; Bushman, D.; Delahoy, M.J.; Currie, D.; Cherney, B.; et al. Performance of an Antigen-Based Test for Asymptomatic and Symptomatic SARS-CoV-2 Testing at Two University Campuses—Wisconsin, September–October 2020. *MMWR Morb. Mortal. Wkly. Rep.* **2021**, *69*, 1642–1647. <https://doi.org/10.15585/mmwr.mm695152a3>.
216. Strömer, A.; Rose, R.; Schäfer, M.; Schön, F.; Vollersen, A.; Lorentz, T.; Fickenscher, H.; Krumbholz, A. Performance of a Point-of-Care Test for the Rapid Detection of SARS-CoV-2 Antigen. *Microorganisms* **2020**, *9*, 58. <https://doi.org/10.3390/microorganisms9010058>.
217. Toptan, T.; Eckermann, L.; Pfeiffer, A.E.; Hoehl, S.; Ciesek, S.; Drosten, C.; Corman, V.M. Evaluation of a SARS-CoV-2 rapid antigen test: Potential to help reduce community spread? *J. Clin. Virol.* **2021**, *135*, 104713. <https://doi.org/10.1016/j.jcv.2020.104713>.

218. Turcato, G.; Zabolli, A.; Pfeifer, N.; Ciccariello, L.; Sibilio, S.; Tezza, G.; Ausserhofer, D. Clinical application of a rapid antigen test for the detection of SARS-CoV-2 infection in symptomatic and asymptomatic patients evaluated in the emergency department: A preliminary report. *J. Infect.* **2021**, *82*, e14–e16. <https://doi.org/10.1016/j.jinf.2020.12.012>.
219. Mak, G.C.K.; Lau, S.S.Y.; Wong, K.K.Y.; Chow, N.L.S.; Lau, C.S.; Lam, E.T.K.; Chan, R.C.W.; Tsang, D.N.C. Evaluation of rapid antigen detection kit from the WHO Emergency Use List for detecting SARS-CoV-2. *J. Clin. Virol.* **2021**, *134*, 104712. <https://doi.org/10.1016/j.jcv.2020.104712>.
220. Zhang, C.; Zhou, L.; Du, K.; Zhang, Y.; Wang, J.; Chen, L.; Lyu, Y.; Li, J.; Liu, H.; Huo, J.; et al. Foundation and Clinical Evaluation of a New Method for Detecting SARS-CoV-2 Antigen by Fluorescent Microsphere Immunochromatography. *Front. Cell Infect. Microbiol.* **2020**, *10*, 553837. <https://doi.org/10.3389/fcimb.2020.553837>.
221. Agulló, V.; Fernández-González, M.; Ortiz de la Tabla, V.; Gonzalo-Jiménez, N.; García, J.A.; Masiá, M.; Gutiérrez, F. Evaluation of the rapid antigen test Panbio COVID-19 in saliva and nasal swabs in a population-based point-of-care study. *J. Infect.* **2021**, *82*, 186–230. <https://doi.org/10.1016/j.jinf.2020.12.007>.
222. Tanimoto, T.; Matsumura, M.; Tada, S.; Fujita, S.; Ueno, S.; Hamai, K.; Omoto, T.; Maeda, H.; Nishisaka, T.; Ishikawa, N. Need for a high-specificity test for confirming weakly positive result in an immunochromatographic SARS-CoV-2-specific antigen test: A case report. *J. Microbiol. Immunol. Infect.* **2021**, *54*, 534–535. <https://doi.org/10.1016/j.jmii.2020.11.004>.
223. Lindner, A.K.; Nikolai, O.; Kausch, F.; Wintel, M.; Hommes, F.; Gertler, M.; Krüger, L.J.; Gaedert, M.; Tobian, F.; Lainati, F.; et al. Head-to-head comparison of SARS-CoV-2 antigen-detecting rapid test with self-collected nasal swab versus professional-collected nasopharyngeal swab. *Eur. Respir. J.* **2021**, *57*. <https://doi.org/10.1183/13993003.03961-2020>.
224. Abdelrazik, A.M.; Elshafie, S.M.; Abdelaziz, H.M. Potential Use of Antigen-Based Rapid Test for SARS-CoV-2 in Respiratory Specimens in Low-Resource Settings in Egypt for Symptomatic Patients and High-Risk Contacts. *Lab. Med.* **2021**, *52*, e46–e49. <https://doi.org/10.1093/labmed/lmaa104>.
225. Weitzel, T.; Legarraga, P.; Iruretagoyena, M.; Pizarro, G.; Vollrath, V.; Araos, R.; Munita, J.M.; Porte, L. Comparative evaluation of four rapid SARS-CoV-2 antigen detection tests using universal transport medium. *Travel Med. Infect. Dis.* **2021**, *39*, 101942. <https://doi.org/10.1016/j.tmaid.2020.101942>.
226. Winkel, B.; Schram, E.; Gremmels, H.; Debast, S.; Schuurman, R.; Wensing, A.; Bonten, M.; Goedhart, E.; Hofstra, M. Screening for SARS-CoV-2 infection in asymptomatic individuals using the Panbio COVID-19 antigen rapid test (Abbott) compared with RT-PCR: A prospective cohort study. *BMJ Open* **2021**, *11*, e048206. <https://doi.org/10.1136/bmjopen-2020-048206>.
227. Hoehl, S.; Schenk, B.; Rudych, O.; Göttig, S.; Foppa, I.; Kohmer, N.; Karaca, O.; Toptan, T.; Ciesek, S. At-home self-testing of teachers with a SARS-CoV-2 rapid antigen test to reduce potential transmissions in schools. *medRxiv* **2020**. <https://doi.org/10.1101/2020.12.04.20243410>.
228. Kannian, P.; Lavanya, C.; Ravichandran, K.; Jayaraman, B.G.; Mahanathi, P.; Ashwini, V.; Kumarasamy, N.; Rajan, G.; Ranganathan, K.; Challacombe, S.J.; et al. Detection of SARS-CoV2 antigen in human saliva may be a reliable tool for large scale screening. *medRxiv* **2020**. <https://doi.org/10.1101/2020.12.17.20248437>.
229. Lindner, A.K.; Nikolai, O.; Rohardt, C.; Kausch, F.; Wintel, M.; Gertler, M.; Burock, S.; Hörig, M.; Bernhard, J.; Tobian, F.; et al. SARS-CoV-2 patient self-testing with an antigen-detecting rapid test: A head-to-head comparison with professional testing. *medRxiv* **2021**. <https://doi.org/10.1101/2021.01.06.20249009>.
230. Filgueiras, P.S.; Corsini, C.A.; Almeida, N.B.F.; Assis, J.V.; Pedrosa, M.L.C.; de Oliveira, A.K.; Amorim, R.N.H.; de Miranda, D.A.P.; Coutinho, L.A.; Gomes, S.V.C.; et al. COVID-19 Rapid Antigen Test at hospital admission associated to the knowledge of individual risk factors allow overcoming the difficulty of managing suspected patients in hospitals COVID-19 Rapid Antigen Test facilitates the management of suspected patients on hospital admission. *medRxiv* **2021**. <https://doi.org/10.1101/2021.01.06.21249282>.
231. Peto, T.; Team, U.C.-L.F.O. COVID-19: Rapid Antigen detection for SARS-CoV-2 by lateral flow assay: A national systematic evaluation for mass-testing. *medRxiv* **2021**. <https://doi.org/10.1101/2021.01.13.21249563>.
232. Jakobsen, K.K.; Jensen, J.S.; Todsén, T.; Lippert, F.; Martel, C.J.-M.; Klokke, M.; von Buchwald, C. Detection of SARS-CoV-2 infection by rapid antigen test in comparison with RT-PCR in a public setting. *medRxiv* **2021**. <https://doi.org/10.1101/2021.01.22.21250042>.
233. Miyakawa, K.; Funabashi, R.; Yamaoka, Y.; Jeremiah, S.S.; Katada, J.; Wada, A.; Takei, T.; Shimizu, K.; Ozawa, H.; Kawakami, C.; et al. SARS-CoV-2 antigen rapid diagnostic test enhanced with silver amplification technology. *medRxiv* **2021**. <https://doi.org/10.1101/2021.01.27.21250659>.
234. Pollock, N.R.; Tran, K.; Jacobs, J.R.; Cranston, A.E.; Smith, S.; O’Kane, C.Y.; Roady, T.J.; Moran, A.; Scarry, A.; Carroll, M.; et al. Performance and Operational Evaluation of the Access Bio CareStart Rapid Antigen Test in a High-Throughput Drive-Through Community Testing Site in Massachusetts. *Open Forum Infect. Dis.* **2021**, *8*, ofab243. <https://doi.org/10.1093/ofid/ofab243>.
235. Shidlovskaya, E.V.; Kuznetsova, N.A.; Divisenko, E.V.; Nikiforova, M.A.; Siniavin, A.E.; Ogarkova, D.A.; Shagaev, A.V.; Semashko, M.A.; Tkachuk, A.P.; Burgasova, O.A.; et al. The Value of Rapid Antigen Tests to Identify Carriers of Viable SARS-CoV-2. *medRxiv* **2021**. <https://doi.org/10.1101/2021.03.10.21252667>.
236. Faico-Filho, K.S.; Finamor Júnior, F.E.; Vinícius Leão Moreira, L.; Lins, P.R.G.; Justo, A.F.O.; Bellei, N. Evaluation of the Panbio™ COVID-19 Ag Rapid Test at an Emergency Room in a Hospital in São Paulo, Brazil. *medRxiv* **2021**. <https://doi.org/10.1101/2021.03.15.21253313>.

237. Schuit, E.; Veldhuijzen, I.; Venekamp, R.; van den Bijllaardt, W.; Pas, S.; Lodder, E.; Molenkamp, R.; GeurtsvanKessel, C.; Velzing, J.; Huisman, R.; et al. Diagnostic accuracy of rapid antigen tests in pre-/asymptomatic close contacts of individuals with a confirmed SARS-CoV-2 infection. *medRxiv* **2021**. <https://doi.org/10.1101/2021.03.18.21253874>.
238. Ducrest, P.J. Development and Evaluation of a new Swiss Made SARS-CoV-2 antigen-detecting rapid test. *medRxiv* **2021**. <https://doi.org/10.1101/2021.03.25.21252280>.
239. Del Vecchio, C.; Brancaccio, G.; Brazzale, A.R.; Lavezzo, E.; Onelia, F.; Franchin, E.; Manuto, L.; Bianca, F.; Cianci, V.; Cattelan, A.; et al. Emergence of N antigen SARS-CoV-2 genetic variants escaping detection of antigenic tests. *medRxiv* **2021**. <https://doi.org/10.1101/2021.03.25.21253802>.
240. Bonde, J.; Ejegod, D.; Pedersen, H.; Smith, B.; Cortes, D.; Leding, C.; Thomsen, T.; Benfield, T.; Schnieder, U.V.; Tingleff, J.; et al. Clinical validation of point-of-care SARS-COV-2 BD Veritor antigen test by a single throat swab for rapid COVID-19 status on hospital patients predominantly without overt COVID symptoms. *medRxiv* **2021**. <https://doi.org/10.1101/2021.04.12.21255299>.
241. Igloi, Z.; Velzing, J.; Huisman, R.; Geurtsvankessel, C.; Comvalius, A.; van Beek, J.; Ensing, R.; Boelsums, T.; Koopmans, M.; Molenkamp, R. Clinical evaluation of the SD Biosensor saliva antigen rapid test with symptomatic and asymptomatic, non-hospitalized patients. *medRxiv* **2021**. <https://doi.org/10.1101/2021.04.21.21255865>.
242. Thell, R.; Kallab, V.; Weinhappel, W.; Mueckstein, W.; Heschl, L.; Heschl, M.; Korsatko, S.; Toedling, F.; Blaschke, A.; Herzog, T.; et al. Evaluation of a novel, rapid antigen detection test for the diagnosis of SARS-CoV-2. *medRxiv* **2021**. <https://doi.org/10.1101/2021.04.22.21255637>.
243. Pollock, N.R.; Berlin, D.; Smole, S.C.; Madoff, L.C.; Brown, C.; Henderson, K.; Larsen, E.; Hay, J.; Gabriel, S.; Gawande, A.A.; et al. Implementation of SARS-CoV2 Screening in K-12 Schools Using In-School Pooled Molecular Testing and Deconvolution by Rapid Antigen Test. *J. Clin. Microbiol.* **2021**, *59*, e0112321. <https://doi.org/10.1128/jcm.01123-21>.
244. Hagbom, M.; Carmona-Vicente, N.; Sharma, S.; Olsson, H.; Jämtberg, M.; Nilsdotter-Augustinsson, Å.; Sjöwall, J.; Nordgren, J. Evaluation of SARS-CoV-2 rapid antigen diagnostic tests for saliva samples. *medRxiv* **2021**. <https://doi.org/10.1101/2021.05.14.21257100>.
245. Thirion-Romero, I.; Guerrero-Zúñiga, S.; Arias-Mendoza, A.; Cornejo-Tjuárez, D.P.; Meza-Meneses, P.; Torres-Erazo, D.S.; Hernández, T.; Galindo-Fraga, A.; Villegas-Mota, I.; Sepúlveda-Delgado, J.; et al. Evaluation of a rapid antigen test for SARS-COV-2 in symptomatic patients and their contacts: A multicenter study. *medRxiv* **2021**. <https://doi.org/10.1101/2021.05.24.21257020>.
246. Chiu, R.Y.T.; Kojima, N.; Mosley, G.L.; Cheng, K.K.; Pereira, D.Y.; Brobeck, M.; Chan, T.L.; Zee, J.S.; Kittur, H.; Chung, C.Y.T.; et al. Evaluation of the INDICAID COVID-19 Rapid Antigen Test in Symptomatic Populations and Asymptomatic Community Testing. *Microbiol. Spectr.* **2021**, *9*, e0034221. <https://doi.org/10.1128/Spectrum.00342-21>.
247. Abusrewil, Z.; Alhudiri, I.M.; Kaal, H.H.; El Meshri, S.E.; Ebrahim, F.O.; Dalyoum, T.; Efrefer, A.A.; Ibrahim, K.; Elfghi, M.B.; Abusrewil, S.; et al. Time scale performance of rapid antigen testing for SARS-CoV-2: Evaluation of 10 rapid antigen assays. *J. Med. Virol.* **2021**, *93*, 6512–6518. <https://doi.org/10.1002/jmv.27186>.
248. Muthamia, E.; Mungai, S.; Mungai, M.; Bandawe, G.; Qadri, F.; Kawser, Z.; Lockman, S.; Ivers, L.C.; Walt, D.; Suliman, S.; et al. Assessment of performance and implementation characteristics of rapid point of care SARS-CoV-2 antigen testing. *medRxiv* **2021**. <https://doi.org/10.1101/2021.06.03.21258290>.
249. Abdul-Mumin, A.; Abubakari, A.; Agbozo, F.; Abdul-Karim, A.; Nuertey, B.D.; Mumuni, K.; Heuschen, A.-K.; Hennig, L.; Denking, C.M.; Müller, O.; et al. Field evaluation of specificity and sensitivity of a standard SARS-CoV-2 antigen rapid diagnostic test: A prospective study at a teaching hospital in Northern Ghana. *medRxiv* **2021**. <https://doi.org/10.1101/2021.06.03.21258300>.
250. Akashi, Y.; Kiyasu, Y.; Takeuchi, Y.; Kato, D.; Kuwahara, M.; Muramatsu, S.; Ueda, A.; Notake, S.; Nakamura, K.; Ishikawa, H.; et al. Evaluation and clinical implications of the time to a positive results of antigen testing for SARS-CoV-2. *J. Infect. Chemother.* **2022**, *28*, 248–251. <https://doi.org/10.1016/j.jiac.2021.10.026>.
251. Lindner, A.K.; Krüger, L.J.; Nikolai, O.; Klein, J.A.F.; Rössig, H.; Schnitzler, P.; Corman, V.M.; Jones, T.C.; Tobian, F.; Gaeddert, M.; et al. SARS-CoV-2 variant of concern B.1.1.7: Diagnostic accuracy of three antigen-detecting rapid tests. *medRxiv* **2021**. <https://doi.org/10.1101/2021.06.15.21258502>.
252. Suliman, S.; Matias, W.R.; Fulcher, I.R.; Molano, F.J.; Collins, S.; Uceta, E.; Zhu, J.; Paxton, R.M.; Gonsalves, S.F.; Harden, M.V.; et al. Evaluation of the Access Bio CareStart™ rapid SARS-CoV-2 antigen test in asymptomatic individuals tested at a community mass-testing program in Western Massachusetts. *medRxiv* **2021**. <https://doi.org/10.1101/2021.06.17.21259109>.
253. Bruins, M.J.; dos Santos, C.O.; Spoelman-Lunsche, M.; van den Bos-Kromhout, M.I.; Debast, S.B. Evaluation of the Panbio™ rapid antigen test for COVID-19 diagnosis in symptomatic health care workers. *medRxiv* **2021**. <https://doi.org/10.1101/2021.06.21.21259234>.
254. Ford, L.; Whaley, M.J.; Shah, M.M.; Salvatore, P.P.; Segaloff, H.E.; Delaney, A.; Currie, D.W.; Boyle-Estheimer, L.; O'Hegarty, M.; Morgan, C.N.; et al. Antigen Test Performance Among Children and Adults at a SARS-CoV-2 Community Testing Site. *J. Pediatric Infect. Dis. Soc.* **2021**, *10*, 1052–1061. <https://doi.org/10.1093/jpids/piab081>.
255. Koskinen, J.M.; Antikainen, P.; Hotakainen, K.; Haveri, A.; Ikonen, N.; Savolainen-Kopra, C.; Sundström, K.; Koskinen, J.O. Clinical validation of automated and rapid mariPOC SARS-CoV-2 antigen test. *Sci. Rep.* **2021**, *11*, 20363. <https://doi.org/10.1038/s41598-021-99886-6>.
256. Nikolai, O.; Rohardt, C.; Tobian, F.; Junge, A.; Corman, V.M.; Jones, T.C.; Gaeddert, M.; Lainati, F.; Sacks, J.A.; Seybold, J.; et al. Anterior nasal versus nasal mid-turbinate sampling for a SARS-CoV-2 antigen-detecting rapid test: Does localisation or professional collection matter? *Infect. Dis.* **2021**, *53*, 947–952. <https://doi.org/10.1080/23744235.2021.1969426>.

257. Stohr, J.J.J.M.; Zwart, V.F.; Goderski, G.; Meijer, A.; Nagel-Imming, C.R.S.; Kluytmans-van den Bergh, M.F.Q.; Pas, S.D.; van den Oetelaar, F.; Hellwich, M.; Gan, K.H.; et al. Self-testing for the detection of SARS-CoV-2 infection with rapid antigen tests. *medRxiv* **2021**. <https://doi.org/10.1101/2021.02.21.21252153>.
258. Bullard, J.; Dust, K.; Funk, D.; Strong, J.E.; Alexander, D.; Garnett, L.; Boodman, C.; Bello, A.; Hedley, A.; Schiffman, Z.; et al. Predicting Infectious Severe Acute Respiratory Syndrome Coronavirus 2 From Diagnostic Samples. *Clin. Infect. Dis.* **2020**, *71*, 2663–2666. <https://doi.org/10.1093/cid/ciaa638>.
259. Cevik, M.; Tate, M.; Lloyd, O.; Maraolo, A.E.; Schafers, J.; Ho, A. SARS-CoV-2, SARS-CoV, and MERS-CoV viral load dynamics, duration of viral shedding, and infectiousness: A systematic review and meta-analysis. *Lancet Microbe* **2021**, *2*, e13–e22. [https://doi.org/10.1016/s2666-5247\(20\)30172-5](https://doi.org/10.1016/s2666-5247(20)30172-5).
260. Dinnes, J.; Deeks, J.J.; Berhane, S.; Taylor, M.; Adriano, A.; Davenport, C.; Dittrich, S.; Emperador, D.; Takwoingi, Y.; Cunningham, J.; et al. Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection. *Cochrane Database Syst. Rev.* **2021**, *3*, Cd013705. <https://doi.org/10.1002/14651858.CD013705.pub2>.
261. Khandker, S.S.; Nik Hashim, N.H.; Deris, Z.Z.; Shueb, R.H.; Islam, M.A. Diagnostic Accuracy of Rapid Antigen Test Kits for Detecting SARS-CoV-2: A Systematic Review and Meta-Analysis of 17,171 Suspected COVID-19 Patients. *J. Clin. Med.* **2021**, *10*, 3493. <https://doi.org/10.3390/jcm10163493>.
262. French, S.D.; McDonald, S.; McKenzie, J.E.; Green, S.E. Investing in updating: How do conclusions change when Cochrane systematic reviews are updated? *BMC Med. Res. Methodol.* **2005**, *5*, 33. <https://doi.org/10.1186/1471-2288-5-33>.
263. Moher, D.; Tsertsvadze, A.; Tricco, A.C.; Eccles, M.; Grimshaw, J.; Sampson, M.; Barrowman, N. When and how to update systematic reviews. *Cochrane Database Syst. Rev.* **2008**, *2008*, Mr000023. <https://doi.org/10.1002/14651858.MR000023.pub3>.
264. Ahmadzai, N.; Newberry, S.J.; Maglione, M.A.; Tsertsvadze, A.; Ansari, M.T.; Hempel, S.; Motala, A.; Tsouros, S.; Schneider Chafen, J.J.; Shanman, R.; et al. A surveillance system to assess the need for updating systematic reviews. *Syst. Rev.* **2013**, *2*, 104. <https://doi.org/10.1186/2046-4053-2-104>.
265. Moher, D.; Tsertsvadze, A.; Tricco, A.C.; Eccles, M.; Grimshaw, J.; Sampson, M.; Barrowman, N. A systematic review identified few methods and strategies describing when and how to update systematic reviews. *J. Clin. Epidemiol.* **2007**, *60*, 1095–1104. <https://doi.org/10.1016/j.jclinepi.2007.03.008>.
266. Elliott, J.H.; Synnot, A.; Turner, T.; Simmonds, M.; Akl, E.A.; McDonald, S.; Salanti, G.; Meerpohl, J.; MacLehose, H.; Hilton, J.; et al. Living systematic review: 1. Introduction-the why, what, when, and how. *J. Clin. Epidemiol.* **2017**, *91*, 23–30. <https://doi.org/10.1016/j.jclinepi.2017.08.010>.
267. Elliott, J.H.; Turner, T.; Clavisi, O.; Thomas, J.; Higgins, J.P.T.; Mavergames, C.; Gruen, R.L. Living Systematic Reviews: An Emerging Opportunity to Narrow the Evidence-Practice Gap. *PLoS Med.* **2014**, *11*, e1001603. <https://doi.org/10.1371/journal.pmed.1001603>.
268. Centers for Disease Control and Prevention Common Investigation Protocol for Investigating Suspected SARS-CoV-2 Reinfection. Available online: <https://www.cdc.gov/coronavirus/2019-ncov/php/reinfection.html> (accessed on 18 May 2022).
269. Centers for Disease Control and Prevention (CDC). Guidance for Antigen Testing for SARS-CoV-2 for Healthcare Providers Testing Individuals in the Community. Available online: <https://www.cdc.gov/coronavirus/2019-ncov/lab/resources/antigen-tests-guidelines.html> (accessed on 4 April 2022).
270. Larremore, D.B.; Wilder, B.; Lester, E.; Shehata, S.; Burke, J.M.; Hay, J.A.; Tambe, M.; Mina, M.J.; Parker, R. Test sensitivity is secondary to frequency and turnaround time for COVID-19 screening. *Sci. Adv.* **2021**, *7*, eabd5393. <https://doi.org/10.1126/sciadv.abd5393>.
271. Arora, S.; Grover, V.; Saluja, P.; Algarni, Y.A.; Saquib, S.A.; Asif, S.M.; Batra, K.; Alshahrani, M.Y.; Das, G.; Jain, R.; et al. Literature Review of Omicron: A Grim Reality Amidst COVID-19. *Microorganisms* **2022**, *10*, 451.
272. Food and Drug Administration. Omicron variant: Impact on Antigen Diagnostic Tests. Available online: <https://www.fda.gov/medical-devices/coronavirus-covid-19-and-medical-devices/sars-cov-2-viral-mutations-impact-covid-19-tests#omicronvariantimpact> (accessed on 28 December 2021).
273. Regan, J.; Flynn, J.P.; Choudhary, M.C.; Uddin, R.; Lemieux, J.; Boucau, J.; Bhattacharyya, R.P.; Barczak, A.K.; Li, J.Z.; Siedner, M.J. Detection of the Omicron Variant Virus with the Abbott BinaxNow SARS-CoV-2 Rapid Antigen Assay. *Open Forum Infect. Dis.* **2022**, *9*, ofac022. <https://doi.org/10.1093/ofid/ofac022>.
274. Salcedo, N.; Nandu, N.; Boucau, J.; Herrera, B.B. Detection of SARS-CoV-2 Omicron, Delta, Alpha and Gamma variants using a rapid antigen test. *medRxiv* **2022**. <https://doi.org/10.1101/2022.01.27.22269299>.
275. de Michelena, P.; Torres, I.; Ramos-García, Á.; Gosalbes, V.; Ruiz, N.; Sanmartín, A.; Botija, P.; Poujois, S.; Huntley, D.; Albert, E.; et al. Real-life performance of a COVID-19 rapid antigen detection test targeting the SARS-CoV-2 nucleoprotein for diagnosis of COVID-19 due to the Omicron variant. *J. Infect.* **2022**, *84*, e64–e66. <https://doi.org/10.1016/j.jinf.2022.02.022>.
276. Stanley, S.; Hamel, D.J.; Wolf, I.D.; Riedel, S.; Dutta, S.; Cheng, A.; Kirby, J.E.; Kanki, P.J. Limit of Detection for Rapid Antigen Testing of the SARS-CoV-2 Omicron Variant. *medRxiv* **2022**. <https://doi.org/10.1101/2022.01.28.22269968>.
277. Deerain, J.; Druce, J.; Tran, T.; Batty, M.; Yoga, Y.; Fennell, M.; Dwyer, D.E.; Kok, J.; Williamson, D.A. Assessment of the Analytical Sensitivity of 10 Lateral Flow Devices against the SARS-CoV-2 Omicron Variant. *J. Clin. Microbiol.* **2022**, *60*, e0247921. <https://doi.org/10.1128/jcm.02479-21>.

-
278. Diederichs, M.; Glawion, R.; Kremsner, P.G.; Mitze, T.; Müller, G.J.; Papies, D.; Schulz, F.; Wälde, K. Is large-scale rapid CoV-2 testing a substitute for lockdowns? *PLoS ONE* **2022**, *17*, e0265207. <https://doi.org/10.1371/journal.pone.0265207>.
279. Mathuria, J.P.; Yadav, R.; Rajkumar. Laboratory diagnosis of SARS-CoV-2—A review of current methods. *J. Infect. Public Health* **2020**, *13*, 901–905. <https://doi.org/10.1016/j.jiph.2020.06.005>.