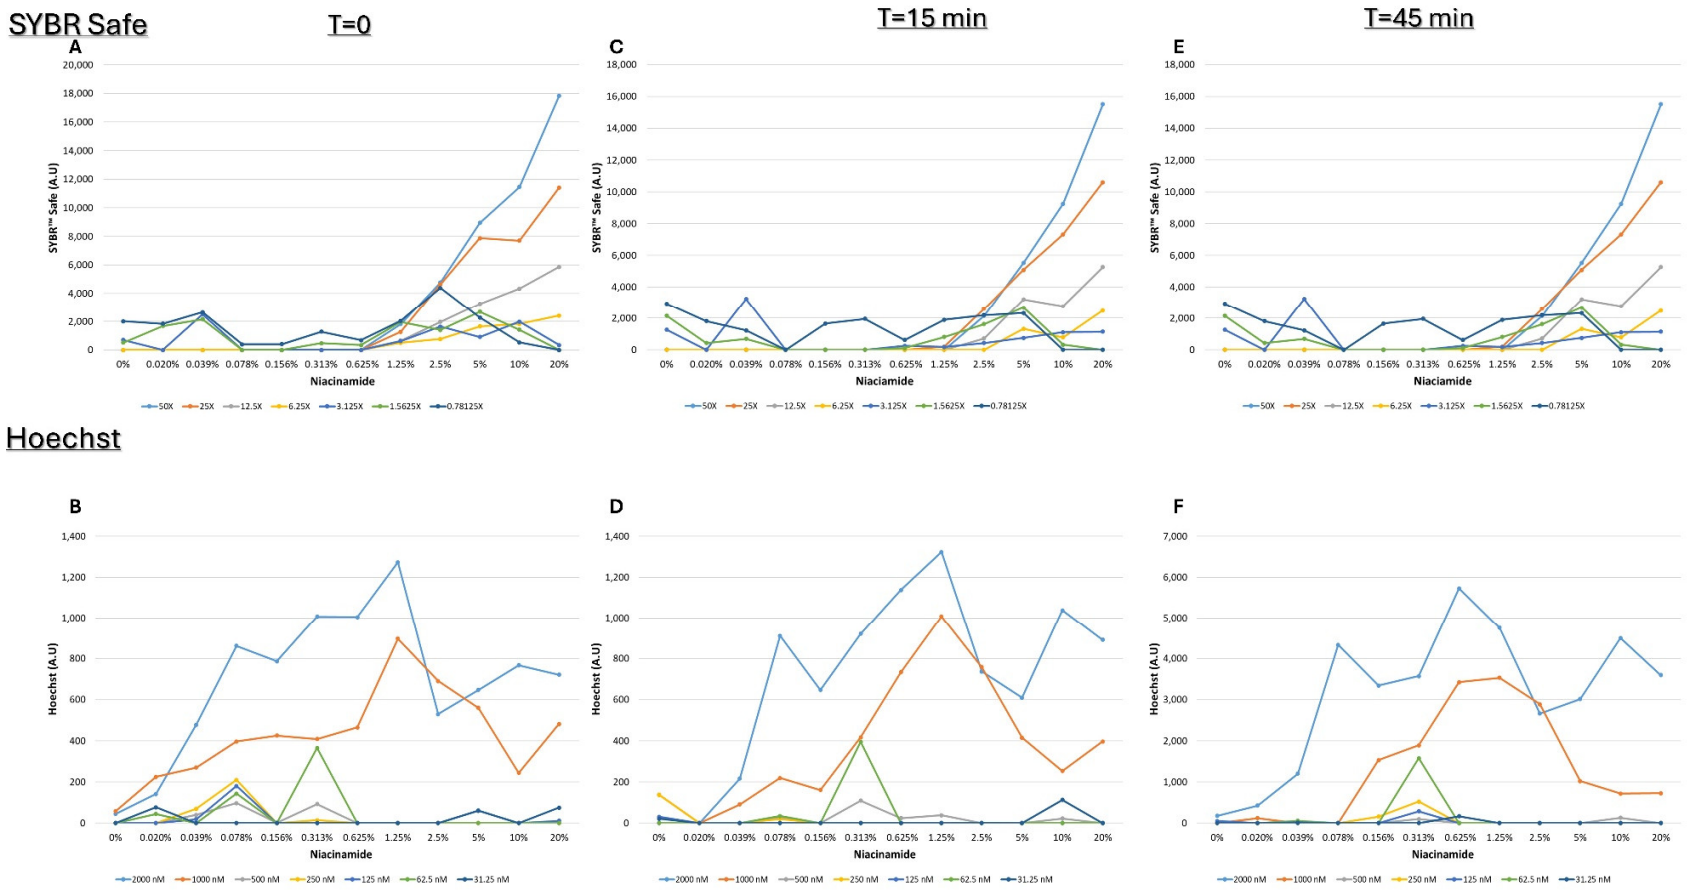


Figure S2. Dye and niacinamide calibration for competition assays. Niacinamide background interaction with DNA intercalating dye SYBR™ safe (A,C,E), and the minor-groove binding dye Hoechst (B,D,F), without DNA was measured at the indicated time points.