

Supplementary Information

Developing a low cost, simple to use electrochemical sensor for the detection of circulating tumour DNA in human fluids

Bukola Attaye ^{1,*}, Chantevy Pou ², Ewen Blair ¹, Christopher Rinaldi ³, Fiona Thomson ², Matthew J. Baker ³ and Damion K. Corrigan ¹

¹ Department of Biomedical Engineering, University of Strathclyde, 40 George Street, Glasgow G1 1QE, UK; ewen.blair@strath.ac.uk (E.B.); damion.corrigan@strath.ac.uk (D.K.C.)

² Wolfson Wohl Cancer Research Centre, Institute of Cancer Sciences, University of Glasgow, Glasgow G61 1QH, UK; Chantevy.Pou@glasgow.ac.uk (C.P.); Fiona.Thomson@glasgow.ac.uk (F.T.)

³ Technology and Innovation Centre, Department of Pure and Applied Chemistry, University of Strathclyde, 99 George street, Glasgow G1 1RD, UK; christopher.rinaldi@strath.ac.uk (C.R.); matthew.baker@strath.ac.uk (M.J.B.)

* Correspondence: bukola.omolaiye@strath.ac.uk

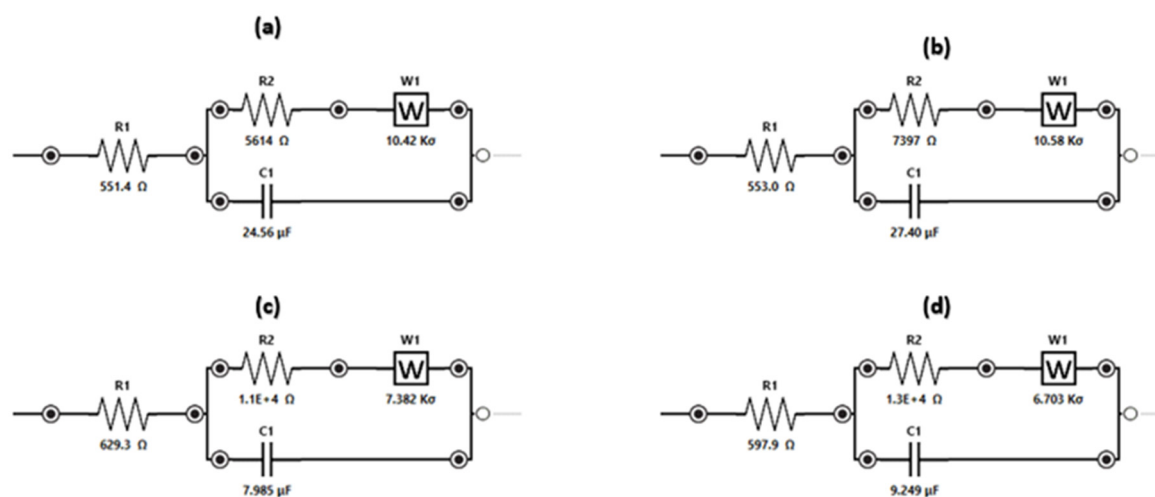


Figure S1. Equivalent circuit models of the impedance spectra recorded for SPCE (a) 25 PCR thermal cycles pre-hybridisation (b) 25 PCR thermal cycles post-hybridisation (c) 30 PCR thermal cycles pre-hybridisation (d) 30 PCR thermal cycles post-hybridisation.