

Erratum

Erratum: Irvine, G.W.; Tan, S.N.; Stillman, M.J. A Simple Metallothionein-Based Biosensor for Enhanced Detection of Arsenic and Mercury. *Biosensors* 2017, 7, 14

Biosensors Editorial Office

MDPI AG St. Alban-Anlage 66, 4052 Basel, Switzerland; biosensors@mdpi.com

Academic Editor: Jeff D. Newman

Received: 14 April 2017; Accepted: 26 April 2017; Published: 5 May 2017

The *Biosensors* Editorial Office wishes to report the following erratum to this paper [1]. In the paper, Figure 6 is the same as Figure 5. The correct version of Figure 6 is as follows:

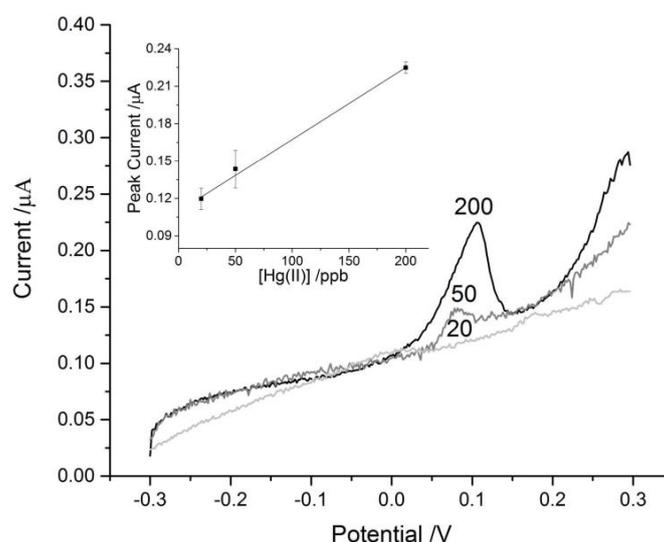


Figure 6. Representative ASV scans of blank paper discs on SPCEs with 25 μL aliquots of Hg^{2+} solutions of concentrations 20, 50 and 200 ppb. The concentration corresponding to each trace is labeled near the peaks at +0.1 V. Inset in the top left corner is the linear fit of the control data ($n = 3$).

The error was introduced during production. We apologize for any inconvenience caused to the readers by this mistake. The manuscript will be updated and the original will remain online on the article website.

References

1. Irvine, G.W.; Tan, S.N.; Stillman, M.J. A Simple Metallothionein-Based Biosensor for Enhanced Detection of Arsenic and Mercury. *Biosensors* **2017**, *7*, 14. [[CrossRef](#)] [[PubMed](#)]



© 2017 by the author. Licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons Attribution (CC BY) license (<http://creativecommons.org/licenses/by/4.0/>).