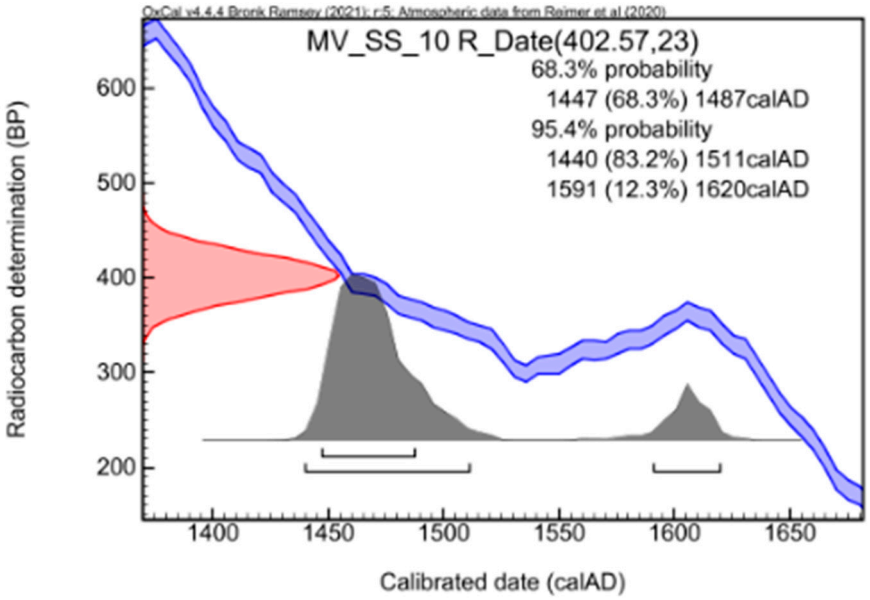


Figure S11. Calibrated dates of the ^{14}C measurements of mortar sample MV_SS_10 by means of OxCal 4.4 [45] and IntCal 20 calibration curve [31].