

Measurement setup

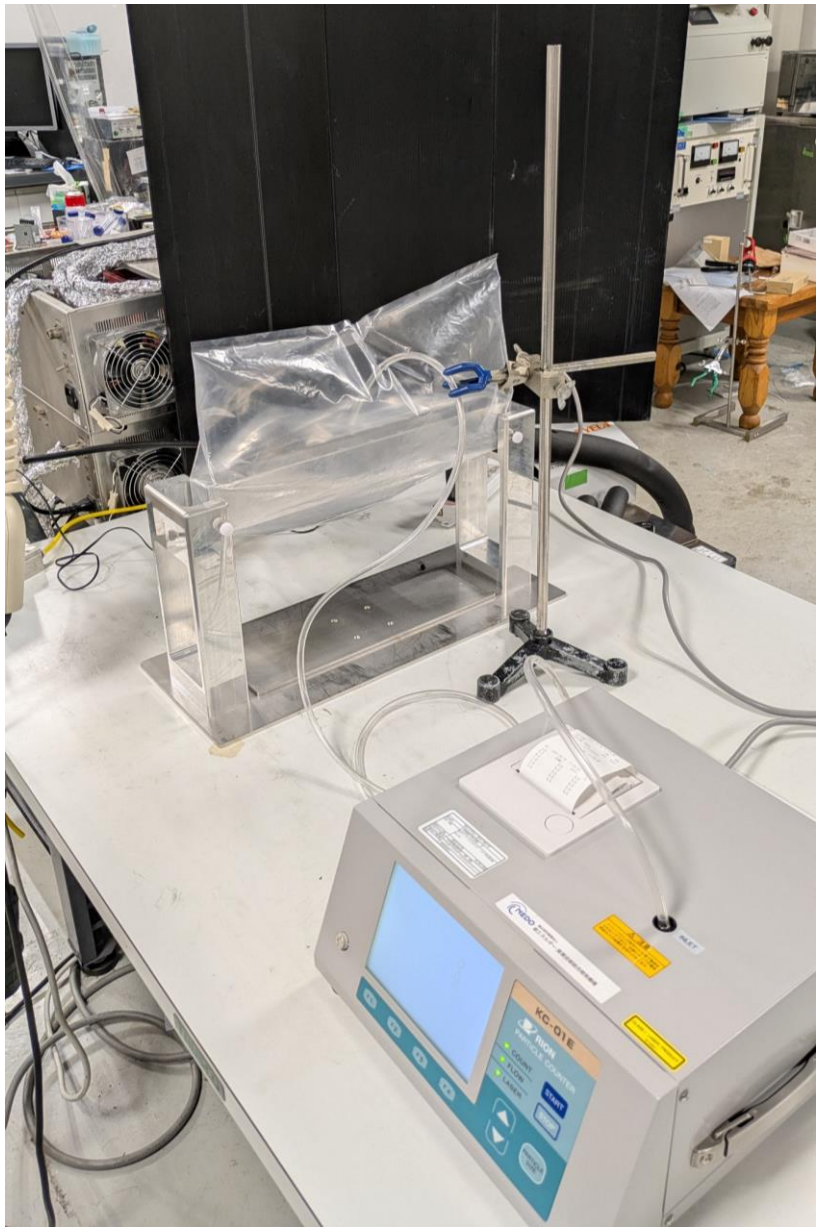

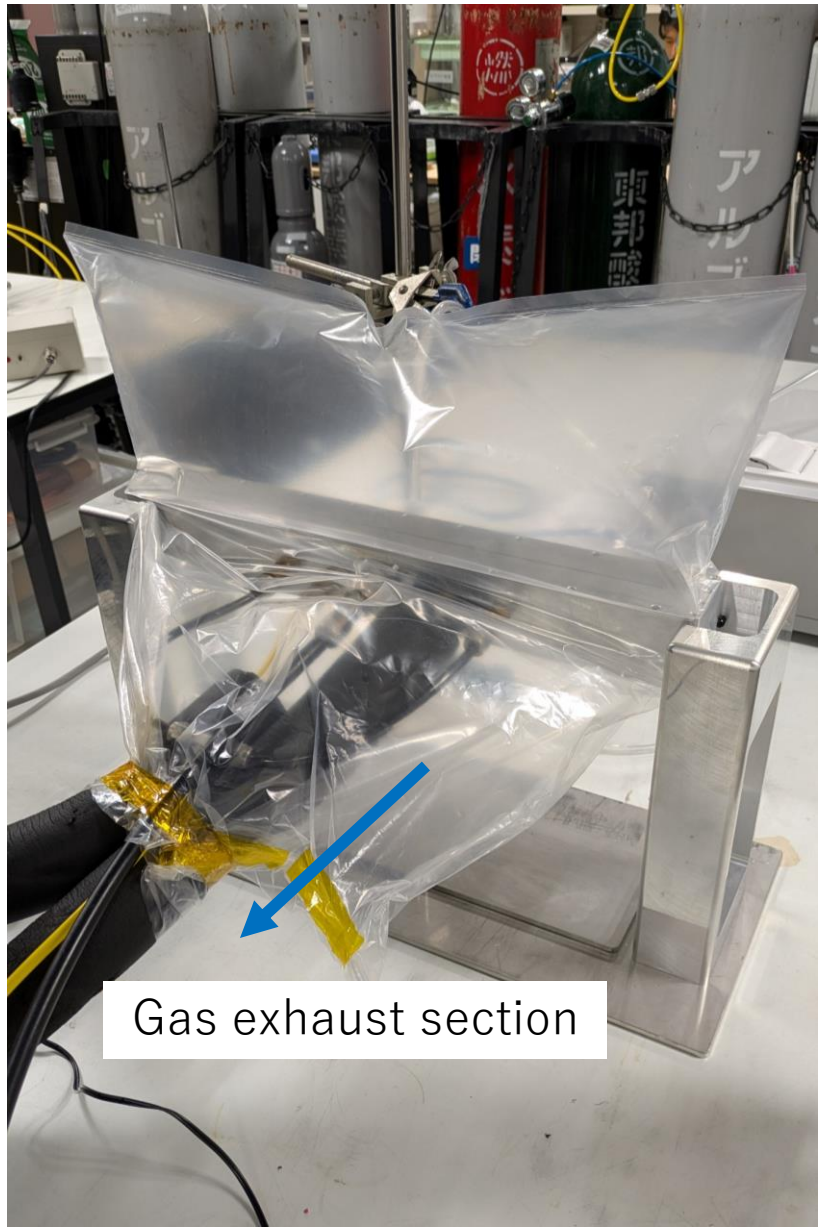

Gas is supplied to the device from a position 40 mm away from the irradiation slit.