

Direct Electron Transfer of Glucose Oxidase on Pre-Anodized Paper/Carbon Electrodes Modified through Zero-Length Cross-Linkers for Glucose Biosensors

Gilberto Henao-Pabon ^{1,†}, Ning Gao ^{2,†}, K. Sudhakara Prasad ^{3,4,†} and XiuJun Li ^{1,3,5,*}

¹ Biomedical Engineering, University of Texas at El Paso, 500 W University Ave, El Paso, TX 79968, USA

² Independent Researcher, 206 via Morella, Encinitas, CA 92024, USA

³ Department of Chemistry & Biochemistry, University of Texas at El Paso, 500 W University Ave, El Paso, TX 79968, USA

⁴ Yenepoya Research Centre, Yenepoya University, Mangalore 575018, Karnataka, India

⁵ Forensic Science & Environmental Science and Engineering, 500 W University Ave, El Paso, TX 79968, USA

* Correspondence: xli4@utep.edu

† These authors contributed equally to this work.

Measurement of spiked human whole blood samples

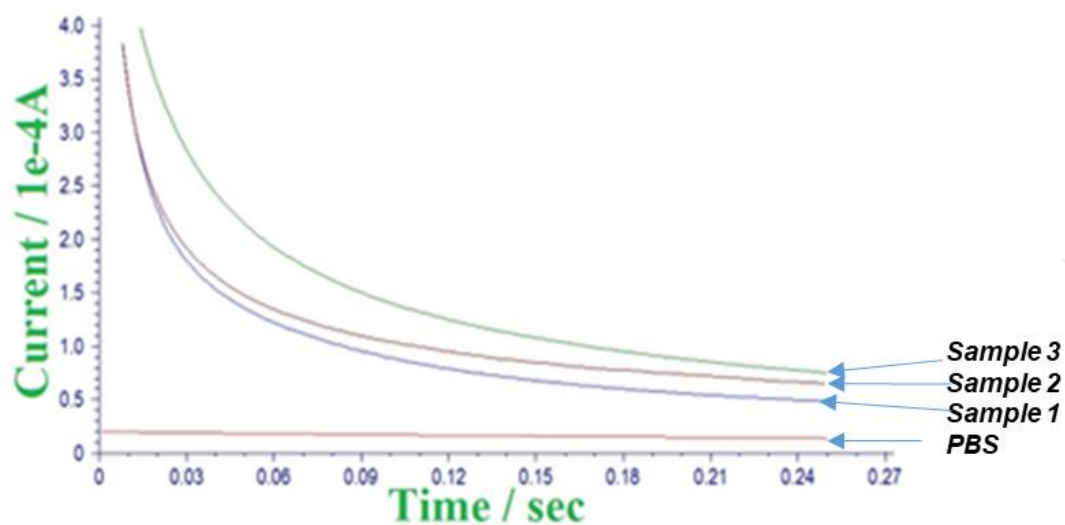


Figure S1. Measurement of human whole blood samples using the paper-based glucose biosensor via direct electron transfer.

Table S1. Glucose measurement results of human whole blood samples (mM).

Glucose	Mean	Mean± Std. Dev.	Std. Error
Sample No. 1	5.9533	5.9533± 0.1721	0.0994
Sample No. 2	7.8353	7.8353± 0.1780	0.1028
Sample No. 3	9.05	9.050± 0.1651	0.0953