

Supplementary material

Pictures from each side of the demonstration model

Figure S1: Facing the rectum (and optional the vagina opening)



Figure S 2: Facing the side of the demonstration model

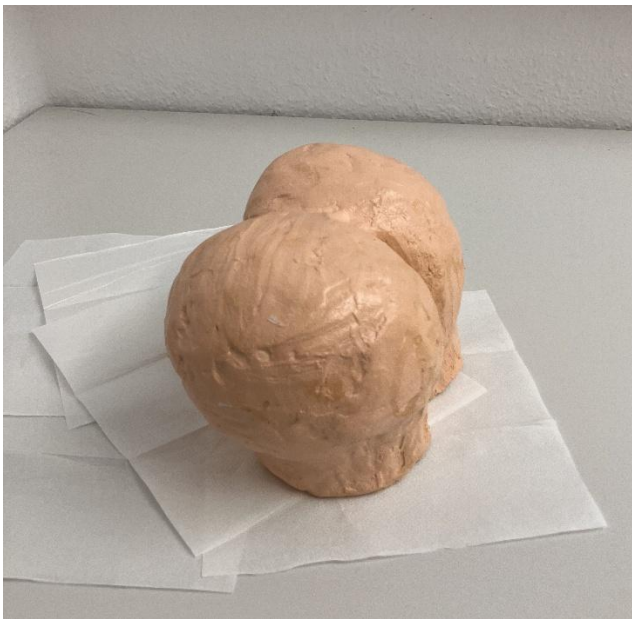


Figure S 3: Facing the tubes (rectal and vaginal openings)



Pictures illustrating the individual steps of the administration

Figure S 4: Push the applicator firmly onto the spout of the spray can



Figure S 5: Shake the spray can before administration



Figure S 6: Twist the dome on top of the spray can

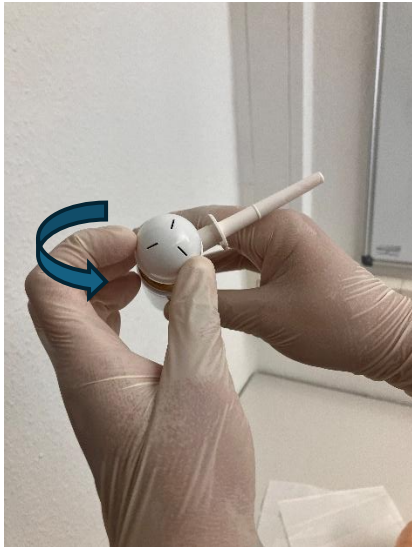


Figure S 7: Turn can upside down



Figure S 8: Hold can with pump dome pointing down during the entire period of administration



Figure S 9: Insert the applicator into the rectum



Figure S 10: Push the pump dome down fully after insertion

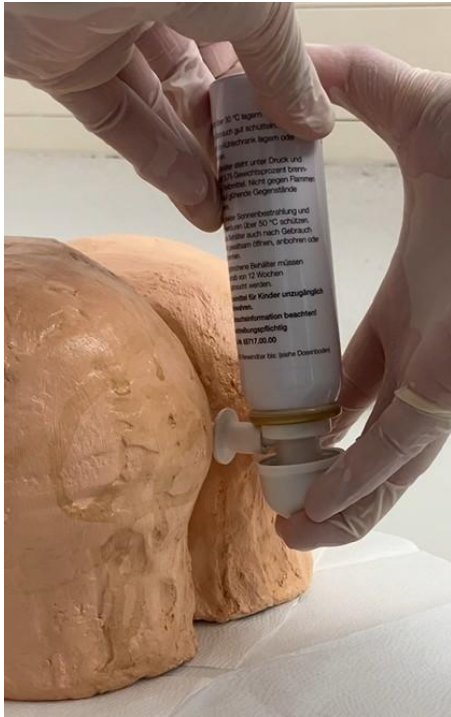


Figure S 11: Release the pump dome slowly after pushing down

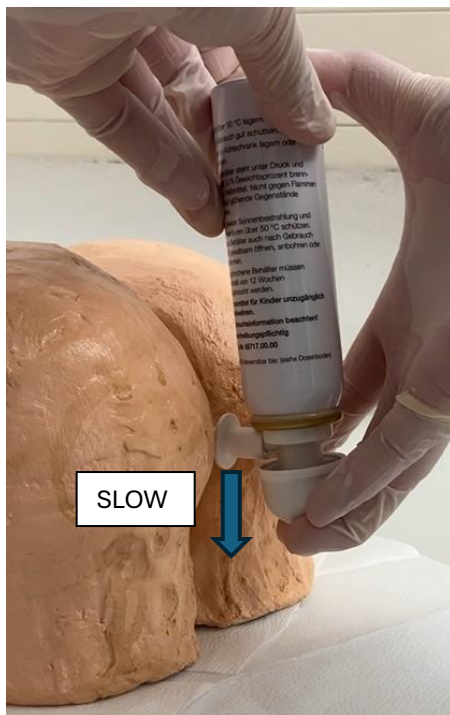


Figure S 12: Take out the applicator from the rectum



Figure S 13: Remove the applicator from the can



Figure S 14: Dispose of the applicator in the plastic bag provided



Figure S 15: Turn back pump dome

