



Supplementary Figure S1. Sample micrographs from used for membrane integrity analysis of *Arapaima gigas* sperm. Sperm smear slides stained with 5% eosin-10% nigrosine and observed under a light microscopy (400X). Spermatozoa with colourless cytoplasm were classified as intact while stained cytoplasm were considered as ruptured.

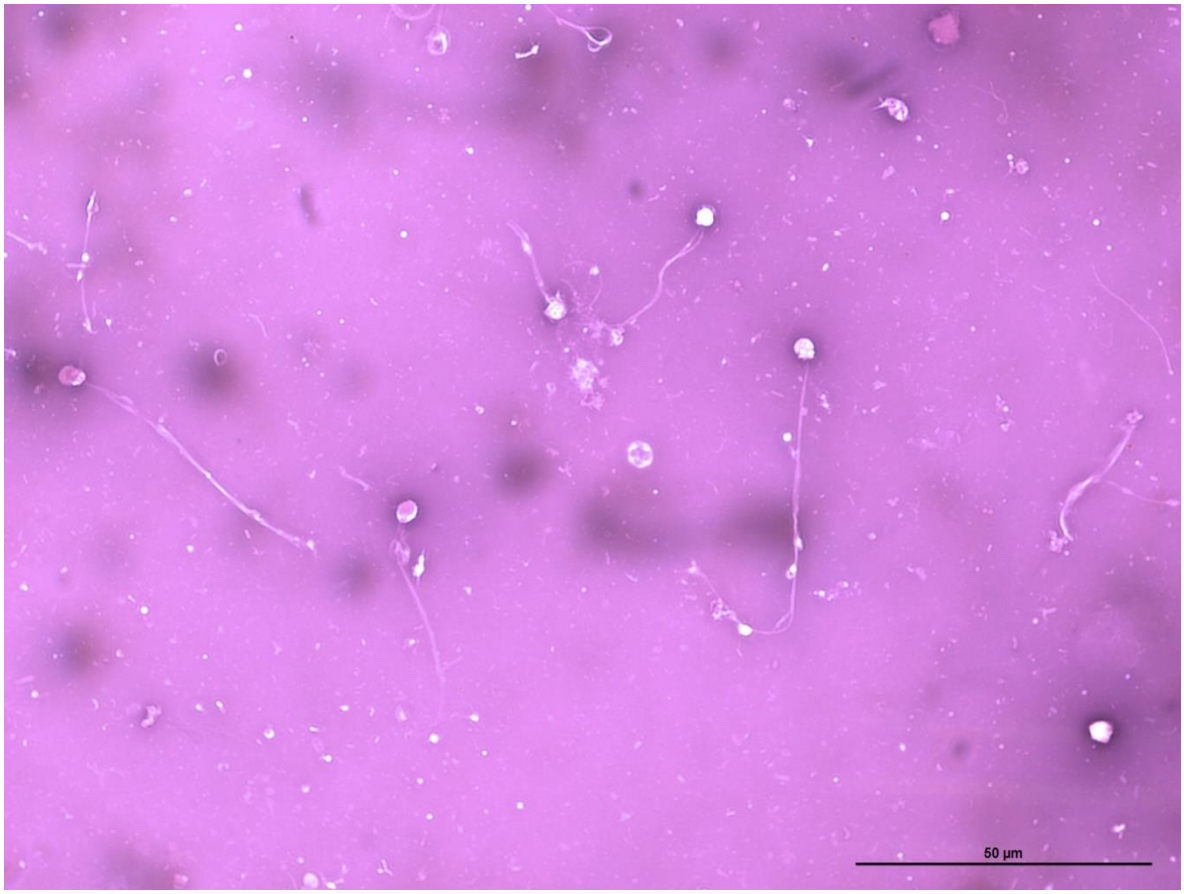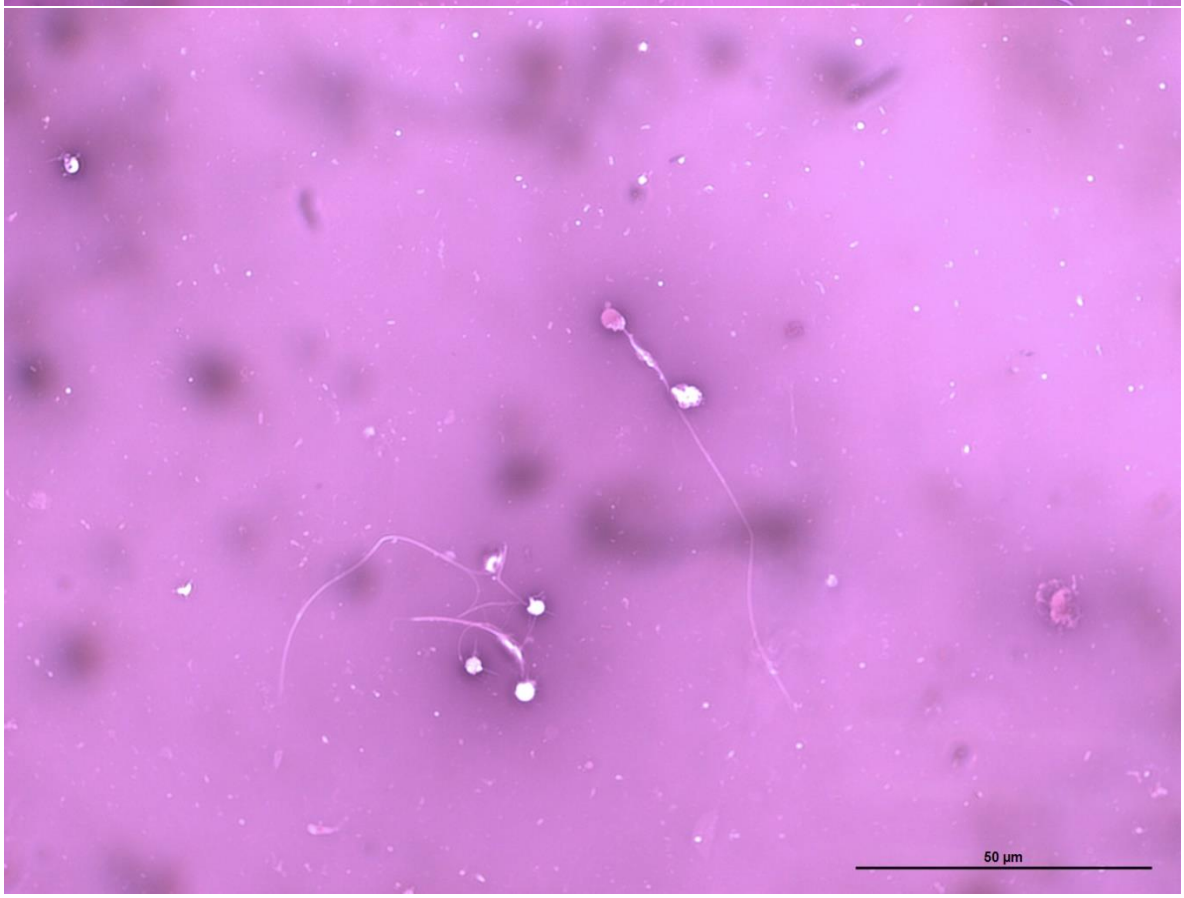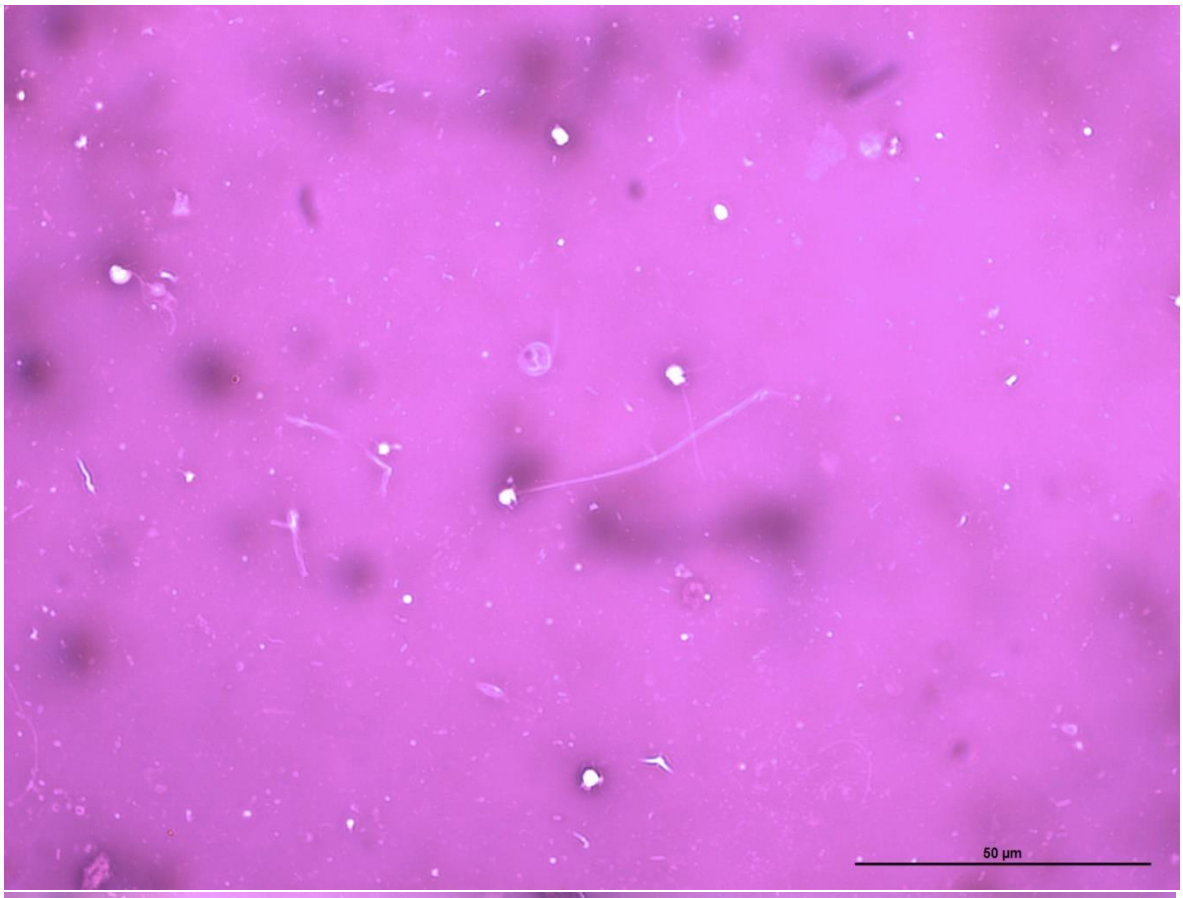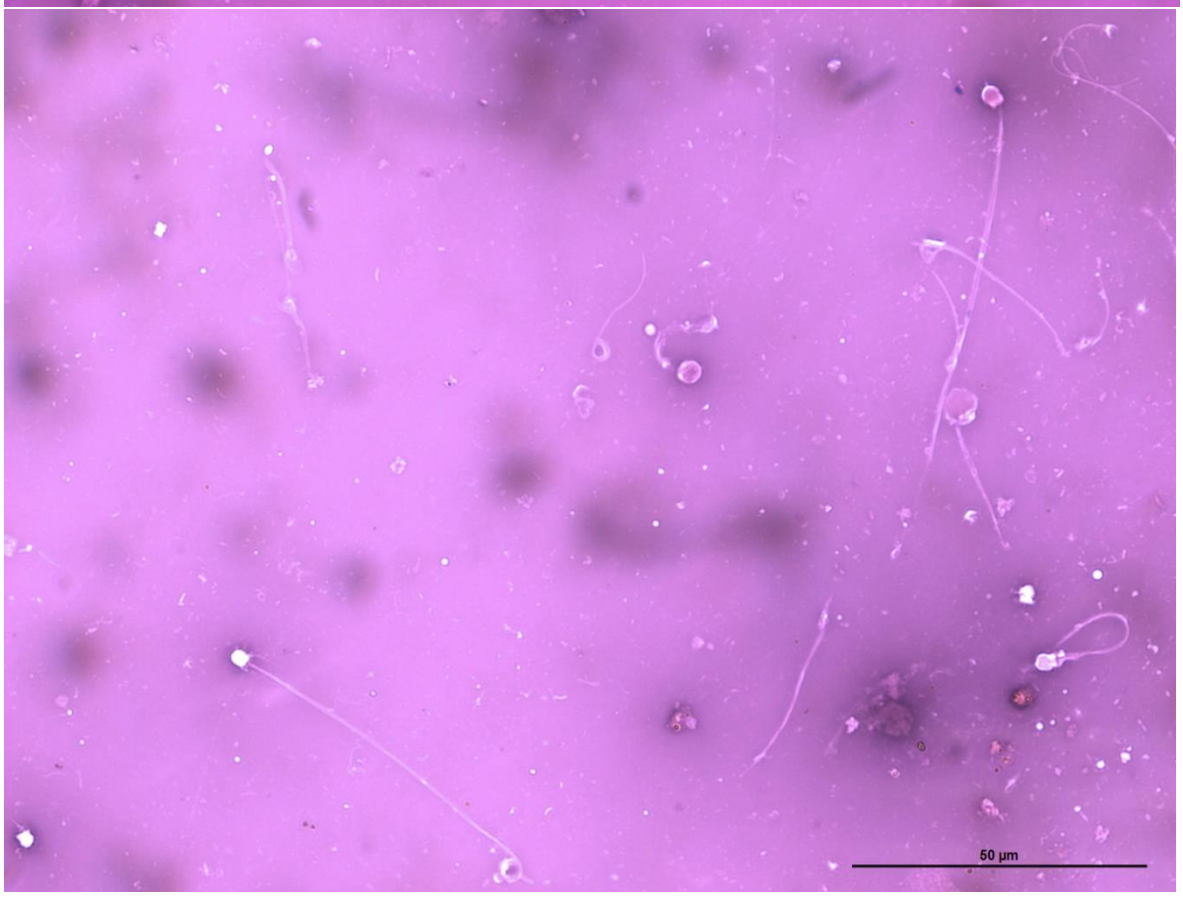


50 µm


50 µm


50 µm


50 µm