Supplementary Materials:

GS-2 was highly effective against Influenza A virus as the addition of GS-2 at only 0 min significantly reduced Influenza A virus by ~2.2 log PFU/mL on ABS coupons ($p < 0.05$, Figure S1). After 15 min and 60 min of GS-2 exposure, Influenza A virus was reduced to below the detection limit, resulting in a >3 log PFU/mL reduction ($p < 0.05$, Figure S1).

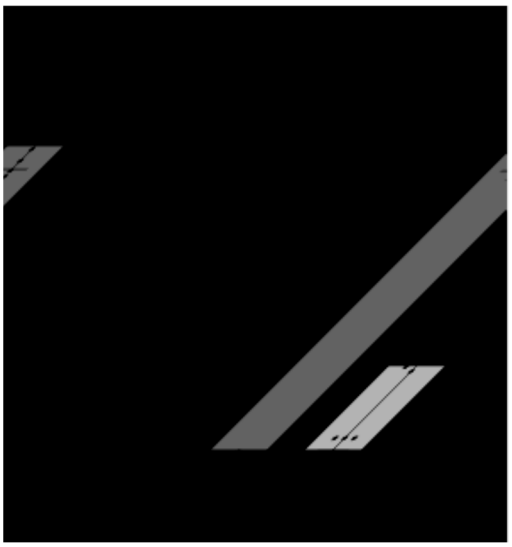


Figure S1: Recovery of Influenza A virus (PFU/mL) with no-GS-2 treatment (control) and 3% GS-2 treatment for 0 (GS-2 + 0), 15 (GS-2 + 15), or 60 (GS-2 + 60) minutes on acrylonitrile butadiene styrene (ABS) coupons. Limit of detection is 2 log PFU/mL. Values are presented as mean ± standard deviation. Asterisks (*) represent significant differences between treatments (GS-2 + 0, GS-2 + 15, or GS-2 + 60 vs. control) on coupon.