


KL-CJ4-006
c13dept135_l.ibk_35 MeOD {D:\u} jic 23

Current Data Parameters
NAME jic-210906-163907_oa
EXPNO 3
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210906
Time 22.36 h
INSTRUM AVIIHD300N
PROBHD Z104275_0359 (
PULPROG deptsp135
TD 98304
SOLVENT MeOD
NS 344
DS 4
SWH 19736.842 Hz
FIDRES 0.401547 Hz
AQ 2.4903679 sec
RG 203.32
DW 25.333 usec
DE 6.50 usec
TE 298.0 K
CNST2 145.0000000
D1 2.00000000 sec
D2 0.00344828 sec
D12 0.00002000 sec
TD0 1
SFO1 75.5088171 MHz
NUC1 13C
P1 9.50 usec
P13 2000.00 usec
PLW0 0 W
PLW1 51.05799866 W
SPNAM[5] Crp60comp.4
SPOAL5 0.500
SPOFFS5 0 Hz
SPW5 7.04050016 W
SFO2 300.2612010 MHz
NUC2 1H
PRG[2] waltz16
PCPD2 12.00 usec
PCPD2 24.00 usec
PCPD2 90.00 usec
PLW2 10.85099983 W
PLW12 0.19291000 W

F2 - Processing parameters
SI 65536
SF 75.5003300 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

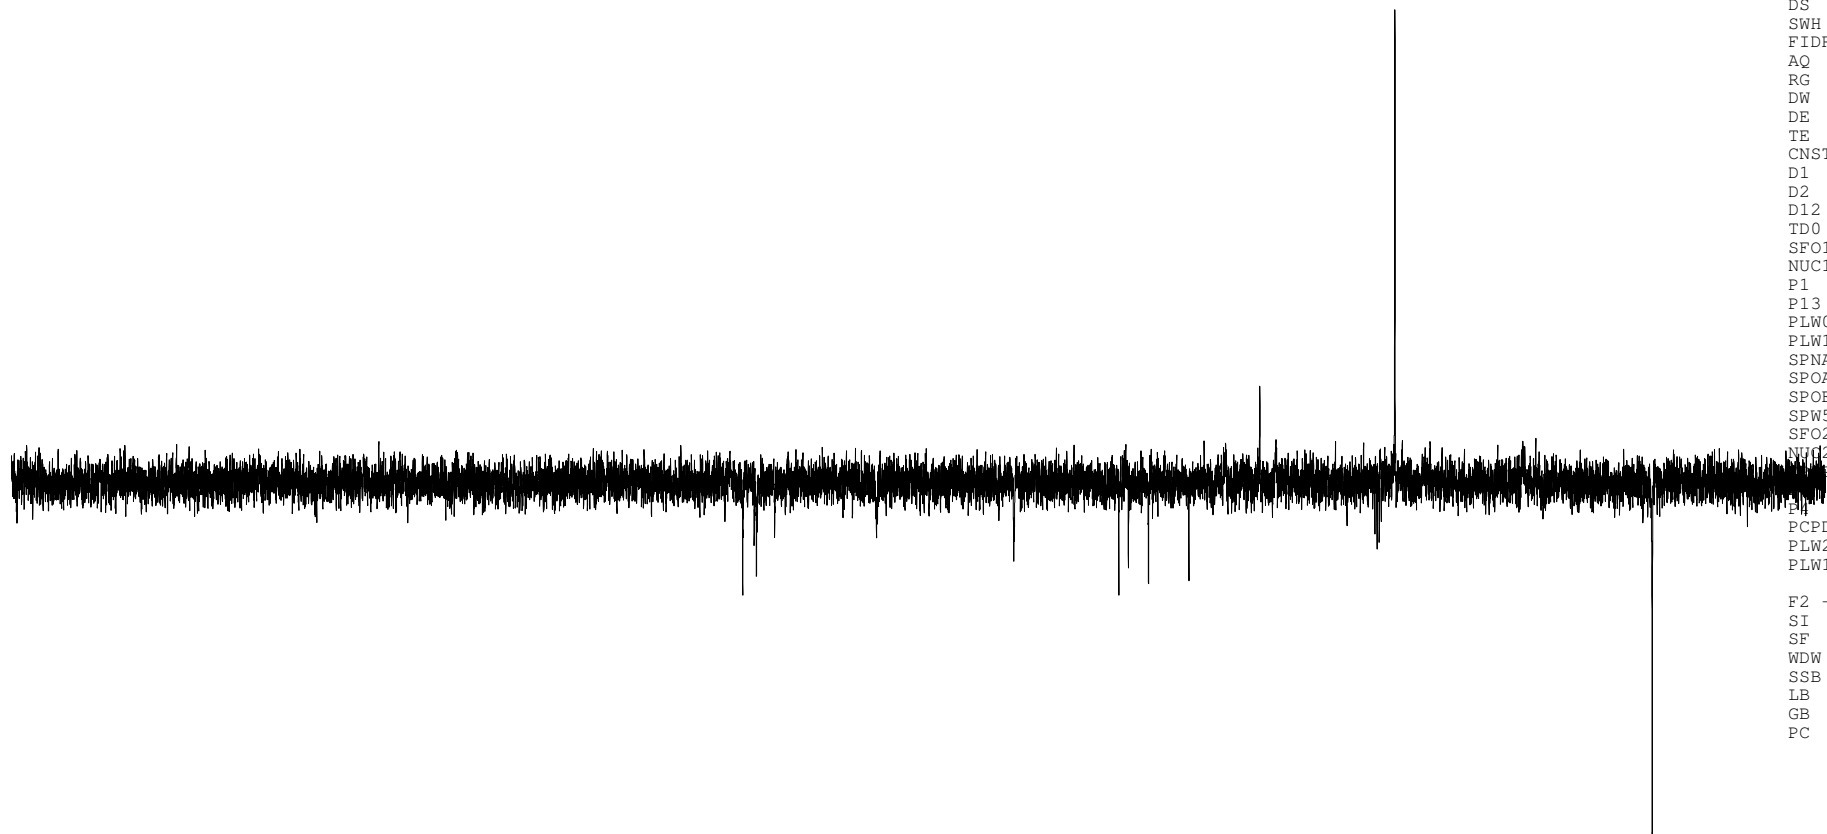

220 210 200 190 180 170 160 150 140 130 120 110 100 90 80 70 60 50 40 30 20 10 0 ppm
F1P: 230 ppm, F2P: -10 ppm
Scale: 10.00 ppm/cm, 755.0 Hz/cm