


KL-CJ4-004
f19cpd.ibk_35 CDCl3 {D:\u} jic 22

Current Data Parameters
NAME jic-210906-163744_oa
EXPNO 4
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210906
Time_ 21.03 h
INSTRUM AVIIHD300N
PROBHD Z104275_0359 (
PULPROG zgfhigqn30.2
TD 262144
SOLVENT CDCl3
NS 40
DS 4
SWH 59523.809 Hz
FIDRES 0.454131 Hz
AQ 2.2020097 sec
RG 203.32
DW 8.400 usec
DE 6.50 usec
TE 298.0 K
D1 2.00000000 sec
D11 0.03000000 sec
D12 0.00002000 sec
TD0 1
SFO1 282.4984248 MHz
NUC1 19F
P0 4.67 usec
P1 14.00 usec
PLW1 8.62240028 W
SFO2 300.2612010 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 10.85099983 W
PLW12 0.19291000 W

F2 - Processing parameters
SI 131072
SF 282.5268000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

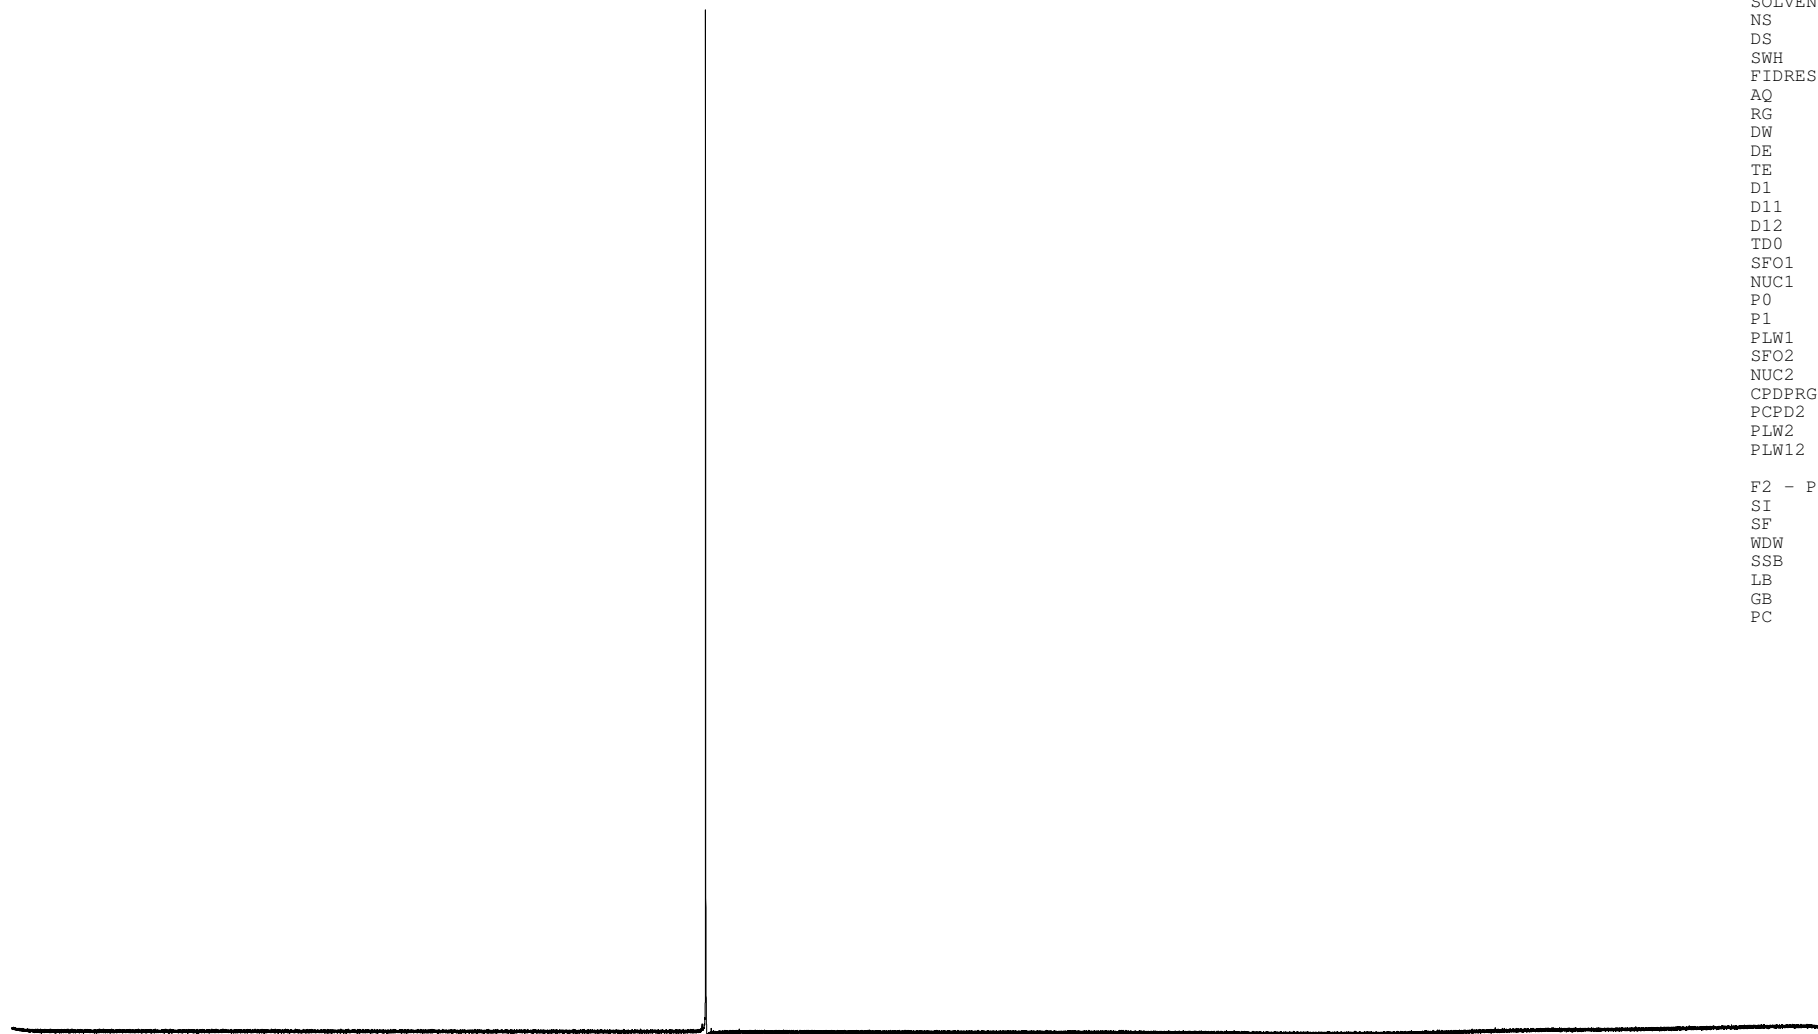

0 -10 -20 -30 -40 -50 -60 -70 -80 -90 -100 -110 -120 -130 -140 -150 -160 -170 -180 -190 ppm
F1P: 5 ppm, F2P: -205 ppm
Scale: 8.750 ppm/cm, 2472 Hz/cm