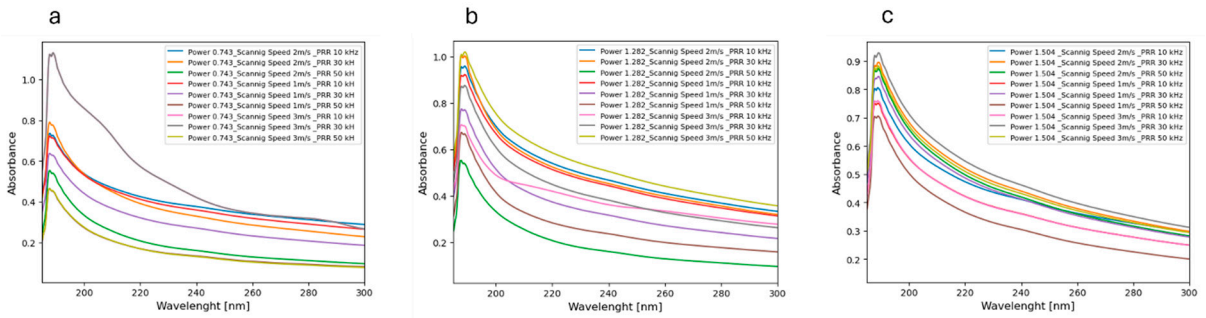


Figure S1. UV-Vis measurement for all the produced samples categorized based on a constant laser power of a) 0.743, b)1.282, and c)1.504 W

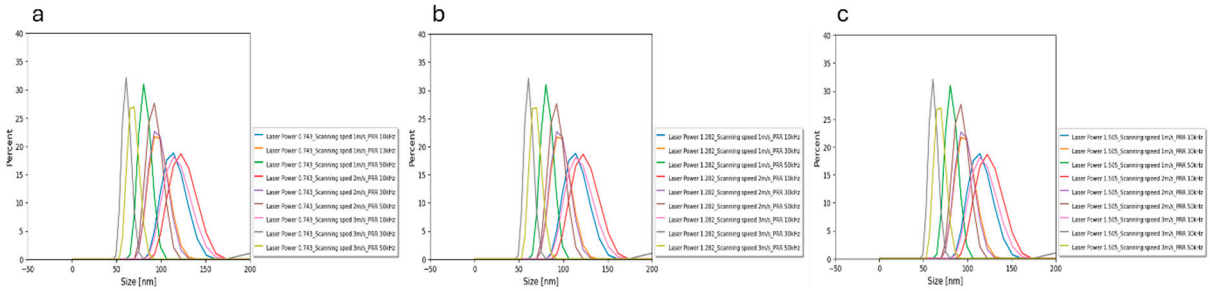


Figure S2. DLS measurement for all the produced samples categorized based on a constant laser power of a)0.743, b)1.282, and c)1.504 W