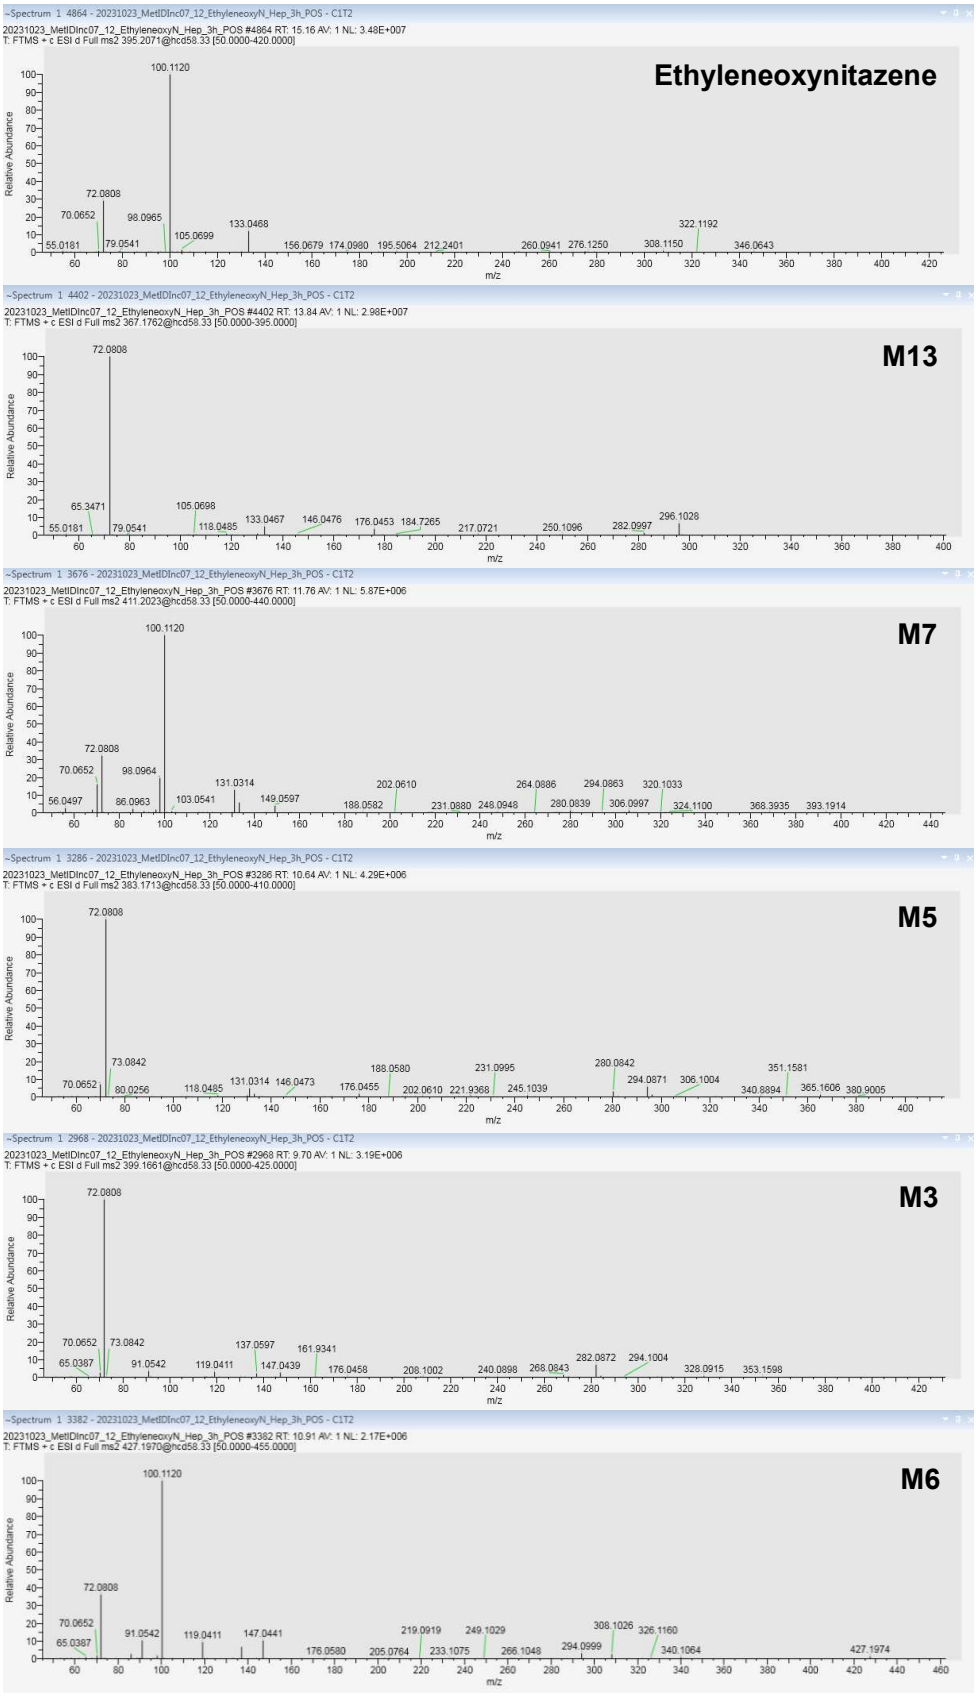

Figure S1. High-resolution tandem mass spectrometry spectra after positive-electrospray ionization of ethyleneoxynitazene and metabolites using the data processing software FreeStyle (v.1.6, Thermo Scientific).