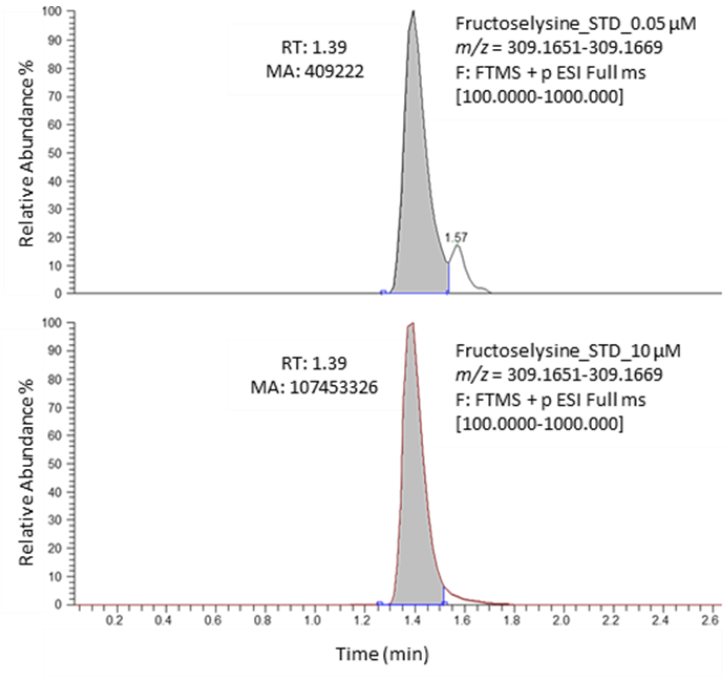


Figure S1. Lowest (LOQ) and highest (ULOQ) concentrations of the FL standard used to build the calibration curve. All chromatograms were acquired with a mass tolerance of 3 ppm.