
S1

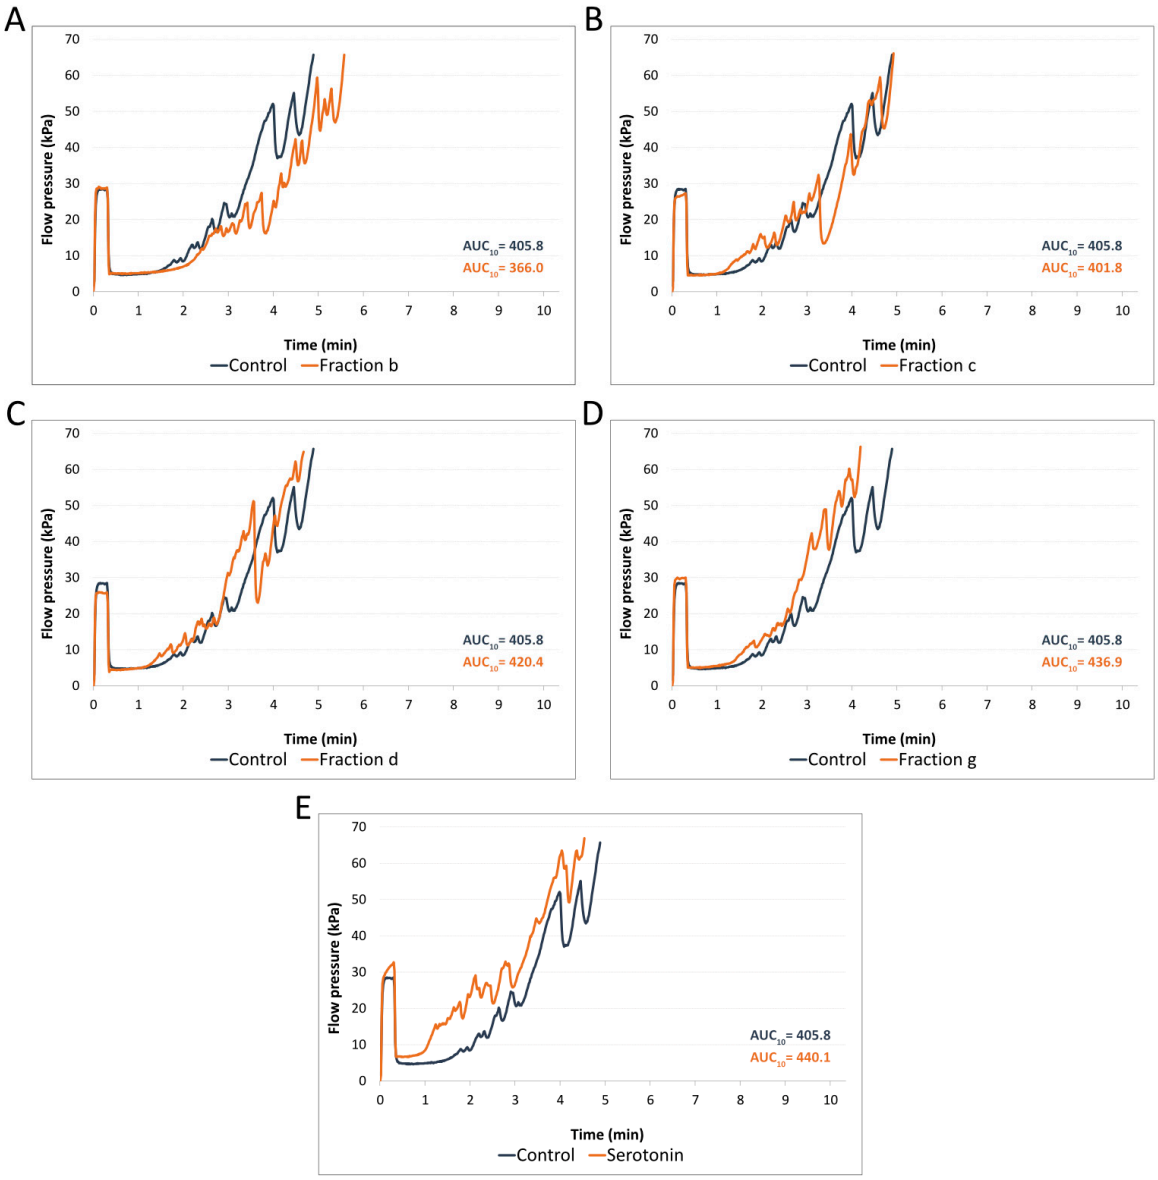

Supplementary Figure S1 (S1). Diagrams of the pressure recorded inside the PL-chip for 10 minutes (or until the occlusion time - 60 kPa), for 50 µg/mL fraction b, c, d, g, and serotonin.